



Photoacoustic Imaging in Medicine – A Review

Mohammed T. GadAllah*, Abd El-Naser A. Mohamed, Alaa A. Hefnawy, Hassan E. Zidan, Ghada M. El-Banby and Samir M. Badawy

KEYWORDS:

Photoacoustic Imaging (PAI), Photoacoustic Tomography (PAT), Multispectral Photoacoustic Tomography (MSOT), Photoacoustic Microscopy (PAM), Raster-Scan Photoacoustic Mesoscopy (RSOM), Photoacoustic Elastography (PAE), Imaging-Guided Surgery (IGS), Non-Contact Laser Ultrasound (LUS).

Abstract — This photoacoustic imaging (PAI) in medicine paper started with an introduction to PAI and the famous photoacoustic techniques including photoacoustic tomography (PAT), multispectral photoacoustic tomography (MSOT), photoacoustic microscopy (PAM), raster-scan photoacoustic mesoscopy (RSOM), and photoacoustic elastography (PAE). A modest review about non-contact laser ultrasound (LUS), having the advantage of operator-independent image quality, has been also demonstrated. A concise review of most of PAI's medical applications is demonstrated including cancer screening (for breast, thyroid, ovarian, prostate, lung, and skin), tissue oxygenation measurements, brain imaging, imaging-guided surgery (IGS), and the guidance of high intensity focused ultrasound (HIFU). Some safety considerations contributed with medical ultrasound and lasers have been then presented. In conclusion, more scientific and clinical development in the field of PAI is expected, and an increase in approved devices that utilize PAI's techniques in medical applications is also expected to serve wide sectors of medicine, whether diagnostic or therapeutic.

I. INTRODUCTION

PHOTOACOUSTIC imaging (PAI), or optoacoustic imaging, is a biomedical hybrid imaging modality based on the use of laser-generated ultrasound due to the photoacoustic effect [1-2]. The photoacoustic effect as a physical phenomenon was reported in 1880 by A. G. Bell [3-6]. The reason is the energy exchange process which transforms the absorbed light energy into kinetic energy, which in role results in a temperature rise thus a pressure wave or sound [6]. Measuring the sound at different wavelengths produced the origin of the photoacoustic spectroscopy (PAS); also, called optoacoustic

spectroscopy (OAS). PAS can be applied to gases, liquids, and solids [6-8]. PAS directly measures the absorbed power of light, which in role serves as a highly sensitive technique with no scattering losses [9]. Photoacoustics' uses have been emerged first in the field of gas spectroscopy and later in biomedical applications [10]. In the last two decades; PAI has rapidly gained wide popularity in more biomedical applications [1]. PAI technique can be roughly expressed as "light in and sound out", merges high-contrast of optical imaging with high spatial resolution and penetration depth of ultrasonography [11-12]. An illustration of the basic principle of PAI is presented in Fig. 1. In PAI: tissue components having different absorption characteristics can be separated spectrally [13]. PAI is sensitive

Received: (28 November, 2021) - Revised: (20 February, 2022) - Accepted: (05 March, 2022)

*Corresponding Author: Mohammed Tarek GadAllah, (Ph.D. Student), Assistant Researcher with Computers and Systems Department, Electronics Research Institute (ERI), Joseph Tito St, Huckstep, El Nozha, Cairo, Egypt. (Emails: mohammed.tag.1986@eri.sci.eg; mohammed.tag.1986@gmail.com)

Abd El-Naser A. Mohamed, Professor Emeritus with Electronics and Electrical Communications Engineering Department, Faculty of Electronic Engineering, Menoufia University, Menoufia, Egypt. (e-mail: abd_elnaser6@yahoo.com)

Alaa A. Hefnawy, Research Professor with Computers and Systems Department, Electronics Research Institute (ERI), Joseph Tito St, Huckstep, El Nozha, Cairo, Egypt. (e-mail: alaa@eri.sci.eg)

Hassan E. Zidan, Researcher with Computers and Systems Department, Electronics Research Institute (ERI), Joseph Tito St, Huckstep, El Nozha, Cairo, Egypt. (e-mail: hbanna@eri.sci.eg)

Ghada M. El-Banby, Associate Professor with Industrial Electronics and Control Engineering Department, Faculty of Electronic Engineering, Menoufia University, Menoufia, Egypt. (e-mail: ghadaelbanby75@gmail.com)

Samir M. Badawy, Professor Emeritus with Industrial Electronics and Control Engineering Department, Faculty of Electronic Engineering, Menoufia University, Menoufia, Egypt. (E-mails: drsamirb@gmail.com; Samir.badawy@el-eng.menofia.edu).

for chromophore mapping, whereas these chromophores can be moreover separated into two categories: the 1st like hemoglobin, melanin, and cytochromes, absorbs ultraviolet-visible light by electronic transitions, while the 2nd like lipids and water, absorbs light ranges from near-infrared to mid-infrared by vibrational transitions [14]. In contrast to conventional ultrasonography, PAI has the potential to produce speckle-free images [3]. Functional information can be provided also by PAI as blood flow, temperature, and oxygenation [2]. Recently, a photoacoustic (PA) topography through an ergodic relay (PATER) system, has been introduced to achieve a wide field of view (FOV), snapshot, and high frame rate in a low-cost system [15-17]. At very deep regions, where PAI cannot achieve adequate resolution, the PA probe should be positioned close to the area of interest by the aid of endoscopy [18]. PA endoscopy is aiming to outdo the resolution limitations of endoscopic ultrasound (EUS) which is a clinically available tomographic tool utilized for diagnosing more diseases [19]. From a market point of view, it is forecasted that the PAI market will increase in 2022 [20].

In this review paper the utilized strategy for achieving it was performing a literature search through the Internet, selecting 189 references to build our review, and contacting with two authors of two different references [71, 111] for giving us permission to process and publish their figures' data.

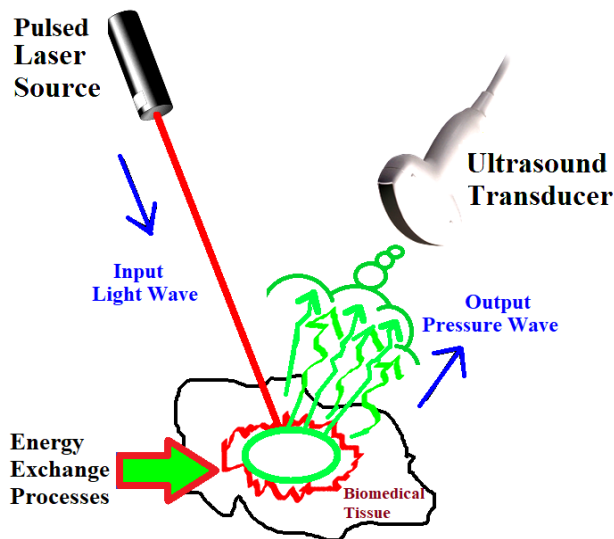


Fig. 1. Illustration of PAI's basic principle.

In the following section II: we will talk about the most famous PA techniques including A. PAT, A.1. MSOT, B. PAM, and C. PAE. In section III, we talk about the recent development of non-contact laser ultrasound (LUS) medical imaging. In section IV, a brief introduction to PAI's applications in medicine mentioned in the following five sections (sections V, VI, VII, VIII, and IX) is presented. In the following section V, most of PAI's applications in cancer screening are presented including A. breast, B. thyroid, C. ovarian, D. prostate, E. lung, and F. skin cancer. Sections VI, VII, VIII, and IX; present in some detail the applications of PAI into tissue oxygenation measurements, brain imaging, Imaging-Guided Surgery (IGS), and PAI's guidance of High Intensity Focused Ultrasound (HIFU), respectively. In section X we will

talk about safety considerations for both laser and ultrasound. Finally, in section XI, we concluded that PAI is a promising biomedical imaging tool in more applications in medicine.

II. MOST FAMOUS PHOTOACOUSTIC STRATEGIES

PAI has more techniques to be implemented. Here, we divided PAI's techniques into five main categories: PAT, PAM, PA endoscopy, PATER, and PAE. A concise chart for the PAI's main techniques mentioned in this paper is illustrated in Fig. 2. Where; OD: optical detection, OR: optical resolution, AR: acoustic resolution, MS: multispectral, fcPAT: functional connectivity PAT, LD: light-emitting diode (LED). In the following sub-sections, we will talk in some detail about A. PAT, B. PAM, and C. PAE. PA endoscopy (the third main category) is a very prospective field in PAI, providing molecular contrast at large depths, allowing for simultaneous visualization of structural and functional information [21]. PA endoscopy presents the same strength in spatial resolution of routinely used clinical EUS, whereas introducing more functional information at physiological sites [22]. For more about PA endoscopy, we refer the reader to [18, 19, 21, 23-28]. PATER (the fourth main category) could be considered a combination of computed PAT theory and PAM, trying to achieve a wide-field image with only a single-element ultrasonic detector upon a single laser shot [15-17]. For more about the PATER technique, we refer the reader to [15-17].

A. PAT

PAT technique can be briefly described in four steps [29, 30]:

1. Illumination of the tissue by a pulsed broad laser beam.
2. A small but rapid temperature rise will be generated.
3. The emitted short-wavelength pulsed ultrasonic waves due to thermoelastic expansion will be then detected by unfocused ultrasonic transducers.
4. Image reconstruction process produces tomographic images of optical contrast and high resolution.

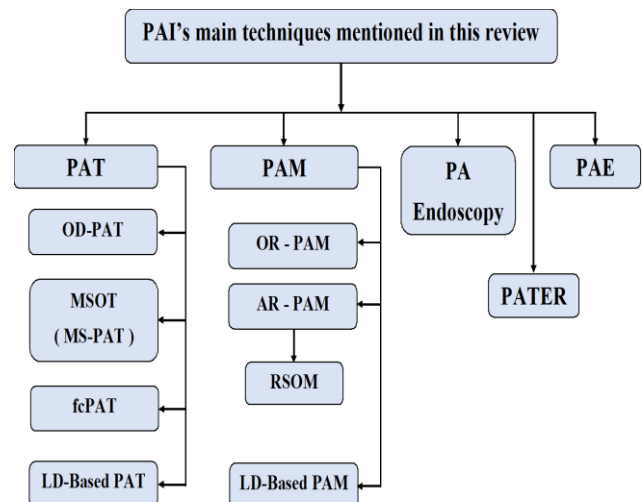


Fig. 2. A concise chart for the PAI's main techniques mentioned in this review.

PAT can image nearly all molecules, fluorescent or not because it doesn't rely on fluorescence emission [31, 32]. PAT is speckle-free unlike ultrasound imaging and optical coherence tomography (OCT) [33]. PAT has the potential to produce fluid-dynamic, functional, molecular, and anatomical imaging, playing an efficient role in biomedical research [34]. PAT has introduced a super-depth combined with high-resolution optical imaging exceeding the optical transport mean free path which is the depth limitation of OCT, confocal microscopy, and two-photon microscopy (~ 1 mm in the skin) [35]. Anatomical and vascular structures imaging can be provided by endogenous hemoglobin contrast. Molecular, functional, and reporter gene imaging can be provided by using exogenous optical contrast [29, 30, 36]. A contrast agent called black mesoporous silicon (BPSi), has been introduced, by Wujun Xu et al [37], for the light-emitting diode (LED) based three-dimensional (3D) PAT, resulting in strong contrast. A United States patent application by James B. Pitner et al [38], has been introduced for Hydroporphyrins as contrast agents for PAI. Another advance to PAT was published by M. Nasiriavanaki et al [39]: developing a functional connectivity photoacoustic tomography (fcPAT) system, allowing non-invasive imaging of the resting-state functional connectivity (RSFC) in a mouse brain, with a large FOV as well as high spatial resolution. RSFC was altered in many brain disorders [39]. A different technique of PAT is the optical-detection photoacoustic tomography (OD-PAT) in which optical approaches have been used to detect the photoacoustic signals instead of piezoelectric detection in classical ultrasound probes [22].

A.1. MSOT

MSOT, a Multispectral PAT (MS-PAT) technique, has been able to introduce a generation of biomedical imaging. A particular advantage of MSOT is its ability to scale with different tissue sizes [40]. MSOT has been succeeded to visualize fluorochromes in tissues that are not visible with conventional single wavelengths' PAI [41]. A fast acquisition MSOT whole-body scanner has been introduced by Rui Ma et al to visualize small animals' molecular markers with multi-wavelength illumination [42]. Razansky et al [43], have introduced their protocol of volumetric real-time MSOT of biomarkers; assuring MSOT's ability in visualizing tissue biomarkers and optical contrast with speed and resolution representative of ultrasound. A fast MSOT platform for dynamic imaging of pharmacokinetics and bio-distribution in multiple organs has been demonstrated by Adrian Taruttis et al [44]; introducing fast and high-resolution in vivo imaging's capabilities. Semi-quantitative MSOT for volumetric Pharmacokinetic (PK) imaging of gastric emptying had been demonstrated by S. Morscher et al; using MSOT in monitoring gastrointestinal motility in mice given indocyanine green (ICG) by oral gavage aiming fate of ICG be monitored in the gastrointestinal tract [45]. Not only ICG, but MSOT also visualize a range of exogenous contrast agents e.g., methylene blue (MB) [46]. The performance of an MSOT system equipped with 2D vs. 3D handheld probes has been demonstrated by Neuschmelting et al [47], for potential clinical translation. First

in vivo clinical use of MSOT non-invasively has been introduced by S. Y. Chuah et al [48], for Structural and functional 3D mapping of skin tumors, confirming the benefit of that imaging method for surgical intervention guidance. Over the last few years, MSOT has succeeded in more than one application in medicine such as imaging of breast cancer [49], particle size-dependent intratumoral distribution of polymeric micelles [50], thyroid disorders [51], drug-induced liver injury (DILI) [52], neural dynamics and organization of the intact mouse brain [53], and orally-administered particles within the gastrointestinal tract of murine models [54]. MSOT has the potential to achieve real-time tracking in vivo of magnetic nanoparticles quantitatively [55]. A co-registration of MSOT and magnetic resonance imaging (MRI) data from murine tumor models, has been introduced by M. Gehrunge et al [56], assuring feasibility of hardware and software-based registration framework for MRI and MSOT images.

B. PAM

PAM technique can be briefly described as focusing a pulsed laser beam into the tissue, ultrasonic waves will be then generated, and finally, a focused ultrasonic transducer will detect the generated waves to form a depth-resolved one-dimension (1D) image [29, 30]. Also, three-dimension (3D) high-resolution tomographic images can be generated by raster scanning [29, 30]. L. V. Wang has illustrated in [57] that: PAM can image up to 3 mm into scattering tissue with 15 micrometers axial resolution while working at 50 MHz ultrasonic detection frequency. Whereas working at 5 MHz, PAM can image ~ 10 times as deep but with ~ 10 times axial resolution [57].

PAM has the potential to image the microvascular network in the skin, which is invaluable in dermatology and related cancer research [58]. Weak acoustic scattering in tissue is an advantage of PAM, unlike pure optical microscopic techniques [59]. PAM breaks through the optical propagation limit (~ 1 mm in soft tissue); providing images with high-resolution at imaging depths up to a few millimeters, with excellent scalability [59].

There are two different techniques of PAM: Optical-resolution photoacoustic microscopy (OR-PAM) and Acoustic-resolution photoacoustic microscopy (AR-PAM).

OR-PAM: this technique uses focused light to spatially limit the stimulation, producing an optical diffraction-limited resolution in the lateral direction.

AR-PAM: in this technique a relatively large area is illuminated, rather than focus light to an optically diffraction-confined spot, so more laser energy is allowed in AR-PAM than in OR-PAM, increasing the chance of photons to reach a much greater depth [22].

In AR-PAM, the illumination can be either **dark-field** or **bright**: The dark-field approach has the advantage to reduce surface interference to deeper PA signals, whereas the bright-field method can carry higher fluence to a targeted volume [22].

A most famous technique that belongs to the AR-PAM family is the **RSOM** (raster-scan optoacoustic mesoscopy).

Optoacoustic mesoscopy is, optoacoustic (or photoacoustic) imaging having acoustic resolution and wide-bandwidth ultrasound detection. RSOM's placement is like a bridge in-between optoacoustic microscopy and optoacoustic macroscopy [60]. Optoacoustic mesoscopy or macroscopy qualifies deeper imaging than optical or optoacoustic microscopy methods which use focused light [46]. A classification of microscopy, mesoscopy, and macroscopy concerning their penetration depth, had been stated by V. Ntziachristos in [61], as: (< 1 mm), (0.5 mm to 10 mm), and (> 1 cm); respectively. Another penetration-based classification had been stated by A. Taruttis, G. M. van Dam, and V. Ntziachristos in [46], as: (< 1 mm), (1–5mm), and (beyond 5 mm); respectively. Over the last decade, more papers have been published concerning optoacoustic mesoscopy [62-69].

In recent years, several applications in medicine have been reported using advanced PAM imaging systems (Such as Laser Diode (LD) based PAM systems) towards a low-cost and aiming for a portable PAM system for point-of-care and wearable applications [70, 71]. LD-based PAM imaging has been investigated to reduce the size of bulky lasers usually used in PAM and also for economic issues [71]. A sample image generated from an original 4060 by 2700 pixels data (taken with permission from [71]) for in vivo LD-based PAM microvasculature imaging of an 8.12 mm by 5.4 mm area from a mouse ear is illustrated in Fig. 3.

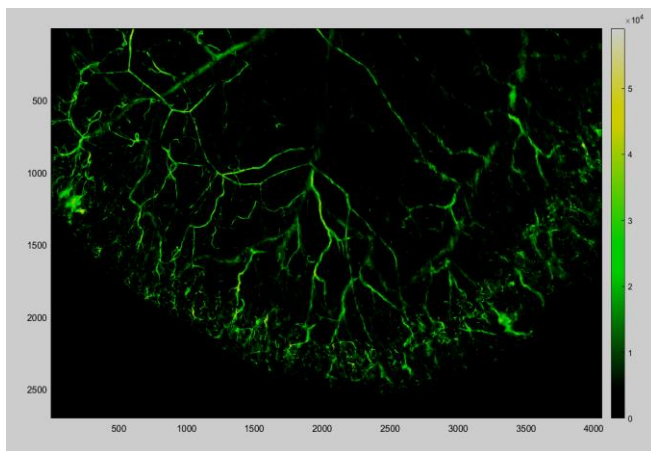


Fig. 3. A sample image produced with permission from [71], illustrating an in vivo LD-based PAM imaging of a mouse ear. Where the numerical values on each X-axis and Y-axis are referring to the pixels' coordinates in the image (where each pixel has a size of $2 \mu\text{m}$ by $2 \mu\text{m}$).

C. PAE

Elastography imaging can be described as art to measure and posterior graphical representation of the spatial allocation of tissue's stiffness [72]. The elasticity distribution in biological tissue can be noninvasively mapped by Elastography to reveal disease conditions [73]. Published studies on PAE imaging (PAEI) are so limited [72]. The start was in 2011, when G. Gao et al, had published their development of a system of PA viscoelasticity imaging, obtaining a high contrast image, reflecting information of the tissue viscoelasticity with the PA

phase projection [74]. In the same year 2011; K. J. Parker et al, have stated their 20 years' perspective on Imaging the elastic properties of tissue [75]. In 2015; Pengfei Hai et al, have proposed Vascular elastic photoacoustic tomography (VE-PAT) to measure blood vessel compliance in humans [76]. A PAT imaging system called quantitative photoacoustic elastography (QPAE) imaging system helping in tissue elastic properties' recovery nondestructively and noninvasively, has been developed by Pengfei et al [72, 77, 78]. Till now, PAE is in the upbringing stage of its development [72].

III. LUS MEDICAL IMAGING

The non-contact laser ultrasound (N-CLUS) medical imaging technique is based on the concept of optical detection of ultrasound (OD-US) [79, 80]. OD-US can play an important role in PAI for biomedical study and clinical diagnosis [80]. In full N-CLUS technique; PA sources are employed on the skin surface, in combination with laser interferometric detection instead of piezoelectric ultrasound detectors used in most PA systems [81]. The main difference between PAI and N-LUS is the detection mechanism (piezoelectric or optical), we can name the technique of N_LUS by optical detection PAI (OD-PAI). Historically, ultrasound generation with lasers nearly goes back to the first laser invention (the ruby laser) [82], which was used for generating ultrasound or shock waves in materials [83]. Recently, more studies have been emerged clarifying the medical applicability of N-CLUS's concept [81-90].

IV. PAI'S APPLICATIONS IN MEDICINE

PAI has a wide variety of applications in more branches in biomedicine [184-189]. In the following sections V, VI, VII, VIII, and IX, a concise review is presented for most PAI's applications in cancer screening, tissue oxygenation measurements, brain imaging, guiding surgeries, and HIFU's guidance, respectively.

V. PAI'S APPLICATIONS IN CANCER SCREENING

In 2020, more than 1.8 million new cancer cases and more than 0.6 million cancer deaths were expected to occur only in the United States [91]. Screening can detect some cancers early when treatment is more often successful [92]. Important elements in cancer control are cancer detection in its early stages and supplying immediate appropriate treatment [93]. PAI can play a role in cancer diagnosis and therapy guidance [94, 95].

A. Breast cancer

A group of diseases in which cells in breast tissue change and divide uncontrolled, typically resulting in a lump or mass, is called breast cancer [96]. Breast cancer is the second common cancer worldwide after lung cancer, the fifth common cause of cancer death [97, 98].

X-ray-based Mammography [97], Breast ultrasound (BUS) imaging [99-101], and Magnetic resonance imaging (MRI) [102, 103], are the three most famous imaging techniques utilized for breast cancer screening. X-ray-based screening mammography, beginning in the 1980s, helps in the early detection of breast cancer [97]. But it uses ionizing radiation, painful breast compression, and has poor performance in radiodense breasts. BUS imaging can be utilized as mammography's adjunct [100, 101]. However, X-ray and BUS imaging are both suffer from having non-optimal sensitivity and specificity [104]. MRI could be used for breast imaging in cases of uncertain findings in X-ray and BUS imaging [104]. However, MRI suffers from limited specificity, requires contrast agents, excludes more patients for instance who have pacemakers, or claustrophobia, moreover it is a little obstructed in premenopausal women by the requirement to time imaging during certain phases of the menstruation cycle [104]. PAI, a nonionizing modality, has the potential to achieve higher specificity in the diagnosis of malignant and benign breast masses, helping to reduce the number of false-positive scans and unnecessary biopsies of benign [104]. Over the last few years, there were various breast' PAI systems have been proposed [105-110]. Recently, Li Lin et al [111], have introduced a high-speed 3D Photoacoustic computed tomography (PACT) system for both preclinical and clinical applications, achieving an in vivo imaging depth of 4 cm in the human breast within a single breath-hold (SBH) of 10 s. Figure 4 is illustrating a sample image of a healthy human subject's right and left breasts in vivo taken by the 3D-PACT system introduced in [111].

B. Thyroid cancer

In 2020, the expected number of new cases of thyroid cancer diagnosed only in the United States (US) is estimated at 52,890. The incidence rate is about 3 times higher in women than in men [92]. Thyroid cancer was the most rapidly increasing cancer in the US till now [92]. In 2012, there were an estimated 40,000 deaths globally due to thyroid cancer [93]. The thyroid gland, normally located in the lower front of the neck, is a butterfly-shaped endocrine gland [112]. Ultrasound combined with fine-needle aspiration cytology (FNAC) is the primary diagnostic tool for thyroid cancer, followed by histology [10]. PAI can augment, FNAC combined ultrasound, for molecular imaging of thyroid nodules. It is because the thyroid gland is superficial (2–3 cm deep) allowing sufficient penetration of light [10]. Recently, more researches have been introduced discussing PAI's utilization in thyroid cancer diagnosis [113-115].

C. Ovarian cancer

In 2020, an expected 21,750 new cases of ovarian cancer will be diagnosed only in the United States and about 13,940 women are expected to die from the disease [92]. Globally, ovarian cancer is the eighth most frequent cause of cancer death among women with 152,000 deaths, as stated by the 2014's world cancer report [93]. Ovarian cancer is rarely detected at an

early stage because of its low spread in the general population [116]. Bin Rao et al, have investigated the feasibility of "optical biopsy", using high OR-PAM to quantify the microvasculature of ovarian and fallopian tube tissue [116]. Through the last decade, there was more than one prototype PAI-based system studying the ability of PAI to enhance ovarian cancer diagnosis [116-119].

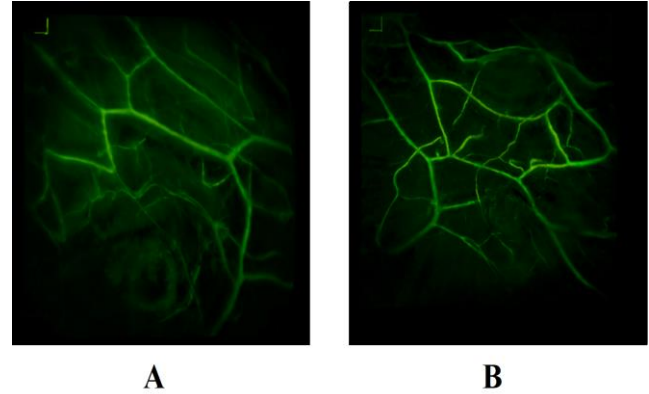


Fig. 4. 3D-PACT of a healthy human subject's breast in vivo (Taken and Processed with permission from [111]). A is a processed perspective angiogram of the Right breast. B is the Left breast image of the same human subject.

D. Prostate cancer

Globally, prostate cancer (PCa) is the second most common cancer in men worldwide [76]. In 2020, the expected new cases of prostate cancer are estimated at 191,930 only in the United States, and 33,330 men are expected to die from the disease [92]. To visualize prostatic anatomy and guide needle biopsy, transrectal ultrasound (TRUS) has been routinely used since the 1980s [120]. A trial in validating if ex-vivo multispectral PAI can characterize malignant prostate tissue, benign prostatic hyperplasia (BPH), and normal human prostate tissue, has been proposed by Dogra et al [121], concluding that multispectral PAI had the potential to differentiate between malignant prostate, BPH and normal prostate tissue. B. L. Bungart et al [122], have published their success in providing prostate biopsy targets by 1064 nm PAT and ultrasonography texture-based feature analysis. Through the last few years, more researches have been emerged concerning enhancing PAI's applications on the prostate [120-125].

E. Lung cancer

Lung cancer is the most frequent cancer worldwide; it is the most common cancer in men and the third in women [93]. As estimated in 2012: there were more than 1.8 million new cases and almost 1.6 million deaths [93]. Only in the United States: the expected new cases of lung cancer in 2020 were estimated at 228,820, whereas the expected mortality from the disease was estimated at 135,720 [92]. Early detection could be a reason for decreasing mortality from lung cancer because most diagnoses occur in a late stage of cancer with a low survival rate [126]. PAI has been studied to help in lung cancer diagnosis

through more than one study during the last decade assuring its promising role in lung cancer diagnosis [126-129].

F. Skin cancer

In recent years, skin cancer cases number has risen globally [1]. Melanoma, Basal cell carcinoma, and squamous cell carcinoma; are the three main types of skin cancer, in which the last two types are called non-melanoma skin cancers (NMSCs) and are seldom life-threatening, whereas the first type: melanoma skin cancers are rare but aggressive and start in pigmented lesions like a mole or birthmark [1]. Nearby lymph nodes are the first site of metastasis where melanoma can spread throughout the body [1]. For precise melanoma prognosis, ascertaining, staging, and planning treatment; the pathological status of the sentinel lymph node is significant [130]. Initial results using PAT by Jose et al [130], suggested that PA could develop into an intraoperative imaging method for detecting melanoma metastases in sentinel lymph nodes. Recently, more researches have been emerged discussing PAI's utilization in skin cancer imaging [131-135].

VI. PAI IN TISSUE OXYGENATION MEASUREMENTS

Oxygen was named by Joseph Priestley and Antoine Lavoisier who had isolated it. Carl Scheele had discovered oxygen in the late eighteenth century. Living cells obtain oxygen through air inhaled into the respiratory system from where it is absorbed into the bloodstream. In red blood cells (RBCs), oxygen is bound to hemoglobin. In some tissues such as muscle, oxygen is also stored bound to myoglobin [136]. William G. K., Peter J. R., and Gregg L. S. have been awarded the 2016 Albert L. basic medical research award for the discovery and clarification of pathways by which humans and other multicellular organisms sense and respond to changes in oxygen availability [137]. The Nobel prize for Physiology or Medicine for 2019 had been given to the same three men for discoveries on the mechanisms by which animals cells respond to changes in oxygen levels [136]. To facilitate blood oxygenation, a specialized oxygen-binding molecule (hemoglobin) is needed since oxygen does not dissolve readily in the plasma because plasma is 93% water [138]. Tissue oxygenation can be imaged by PA based on the oxygen-dependent light absorption characteristics of hemoglobin [139]. Molar extinction coefficient (cm-1/M) spectra curves for HBO2 and HB are shown in Fig. 5. Where: M is referring to the molar concentration in moles/liter. Where HbO2 (red): refers to Oxygenated Hemoglobin, and HB (blue): refers to Deoxygenated Hemoglobin.

Oxygen saturation (sO2) can be described by equation (1) taken from [138]; Where THb: refers to Total Hemoglobin Concentration.

$$sO2 = HbO2/THb \quad ; \quad THb = HbO2 + Hb \quad (1)$$

Blood oxygenation measurements by PAT are an important application been widely carried out in PA studies of tumor hypoxia, brain functions, cancer therapy, and wound healing [140]. PAM has been able to image sO2 in the microvasculature of biological tissues [141]. PAI can deduce the spatial allocation of sO2 in blood, and be co-registered with ultrasonography images of the surrounding anatomy [142]. sO2 can be expected from the partial pressure of blood's oxygen (pO2) based on a standard dissociation curve shown in [142]. Real-time assessment of tissue hypoxia in vivo can be achieved by combining PA and high-frequency ultrasound [143]. In blood flow measurements, PAI has an efficient role [144-146].

VII. PAI IN BRAIN IMAGING

The absorption spectra of deoxyhemoglobin (Hb) and oxyhemoglobin (HbO2) enabled PAT to provide label-free functional brain images of oxygen saturation (sO2) and total hemoglobin concentration (THb) [13]. For improving the visibility of the neurovascular structures, optical contrast agents, like nanoparticles and organic dyes can be used [13]. Different PAI brain imaging techniques have emerged through the last few years [13, 147]. Visualizing Alzheimer's disease of a mouse's brain has been reported by Park SJ et al [148], applying the MSOT technique utilizing an optical imaging probe (CDnir7: Compound of Designation near-infrared 7). Recently, more researches have been emerged discussing different types of PAI schemes, techniques, and applications in brain imaging [148, 149-162].

VIII. PAI IN IMAGING-GUIDED SURGERY (IGS)

Imaging-guided surgery (IGS) is a branch of the concept of Image-guided therapy (IGT) which includes any intervention or surgery that utilizes improved imaging for monitoring, localizing, controlling, and targeting procedures [163]. Due to PAI's ability in noninvasive diagnosis of various types of tissues including bone: PAI could be applied in IGS providing real-time visualization and analysis abilities during more than one type of surgery, for instance: cancer surgery and spinal surgery, helping surgeons in avoiding pedicle breaches by choosing an adequate starting point before drilling or pedicle probe insertion [164]. An intraoperative breast cancer screening by PA has been demonstrated by Ivan K. et al [165], producing a new perspective for malignant cancer visualization moreover surgical guidance. In 2020, a United States patent by M. Bell et al has been dated for a system and method of transcranial PAI to guide skull base surgeries [166]. For more about PA-guided surgery, we refer the reader to [167].

IX. PAI'S GUIDANCE OF HIFU

Providing non-invasive heating and ablation for a wide range of applications, HIFU was rapidly obtaining clinical approval with only a single session required usually for

treatment (day case procedure) [168]. An integrated HIFU drive system on a chip has been introduced by Omid F. et al [169], proposing the feasibility of their system of HIFU based integrated catheter ablation that containing a drive signal generator integrated circuit (IC), and a capacitive micromachined ultrasound transducer (CMUT) ring array. Since, Tumors in organs partially becloud by the rib cage are a challenge for HIFU therapy because of HIFU's beams distortion reducing the focusing gain at the target, Mohamed A.

and Emad E. have introduced a new method of refocusing that can steer power towards the target, whereas limiting the deposition of power on the ribs using the semidefinite relaxation (SDR) technique in approximating the original (non-convex) optimization problem [170]. Through the last few years, more researches have emerged concerning the applications of combining PAI and HIFU [171-174].

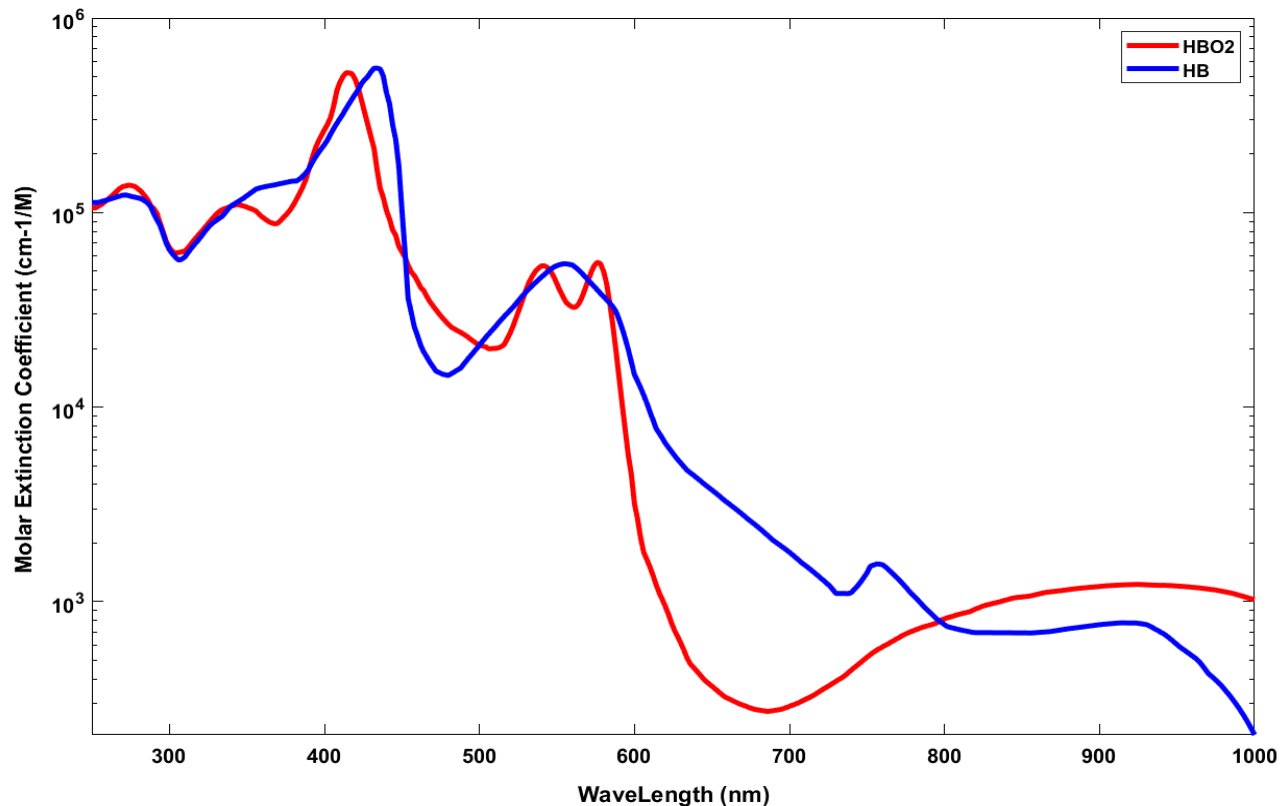


Fig. 5. Molar extinction coefficient (cm-1/M) spectra curves for HBO2 (red) and HB (blue) through different wavelengths (nm). Where: M is referring to the molar concentration in moles/liter (The raw data for these two curves have been taken from: <https://omlc.org/spectra/hemoglobin/summary.html>).

X. SAFETY CONSIDERATIONS

In most traditional ultrasound imaging the ultrasound probe does a dual job: transmitting and receiving ultrasound in both directions as shown in Fig. 6 – A, so more studies concerning ultrasound safety have been emerging concerning this topic, however, diagnostic ultrasound has been widely accepted with an impressive safety record since the 1950s [175-176]. For more about the factors contributing to this record, ultrasound thermal and non-thermal or mechanical (cavitation) induced bio-effects, ultrasound safety considerations, and exposure practice and levels; we refer the reader to [176 – 181].

In PAI: the existence of ultrasound is just the output from the biological tissue due to the PA effect and the ultrasound probe is just utilized for receiving the induced ultrasound waves as illustrated in Fig. 6 -B, so the ultrasound safety consideration illustrated is not applicable here in PAI's. Instead, Laser safety

is so important in PAI. In PAI the used laser type, class, and exposure limit must be included in the safe range standards of the laser. laser's safety standards for use vary in their scope and design, for more about international standards for using laser, American National Standards Institute (ANSI) standards for using laser, laser safety exposure limits, and laser hazard classification classes we refer the reader to [182]. Wherever it is located, a laser is as safe or as hazardous as the user; hence, well and safely a clinical practice operates can be defined by the user's knowledge and skill [183].

XI. SUMMARY AND CONCLUSION

Photoacoustic Imaging (PAI) has wide applications in medicine. There are more techniques of PAI including; PAT,

MSOT, fcPAT, OD-PAT, OR-PAM, AR-PAM, RSOM, PA endoscopy, PATER, and PAE. In the last two decades: the medical applications of photoacoustics have been widely spread. In cancer diagnosis; PAI has a big role, for instance in cancers detection of breast, thyroid, prostate, and skin. Visualizing Alzheimer's disease could be possible by PAI's Brain imaging. PAI could help in a real-time assessment of tissue hypoxia. PAI's guidance plays a strong role in more applications of IGS and HIFU. Our conclusion is the expectation of more future applications of PAI in medicine. Moreover, OD-PAI or N-CLUS, LED-based PAI, PATER, and PA endoscopy systems can generate promising techniques opening the door for more researches in this field.

ACKNOWLEDGEMENTS

- 1- Authors hereby thank Dr. Terence T. W. Wong, and Xiufeng Li, for providing the original data of their paper [71] to us and giving us permission to process and publish. Also, thanks to the rest co-authors of [71]: Victor T. C. Tsang, Lei Kang, and Yan Zhang.
- 2- Authors hereby thank Prof. Dr. Lihong V. Wang, for providing us a permission to process and publish the original breast figure's data of his paper: [111]. Also, thanks to the rest co-authors of [111]: Li Lin, Peng Hu, Xin Tong, Shuai Na, Rui Cao, Xiaoyun Yuan, David C. Garrett, Junhui Shi, and Konstantin Maslov.

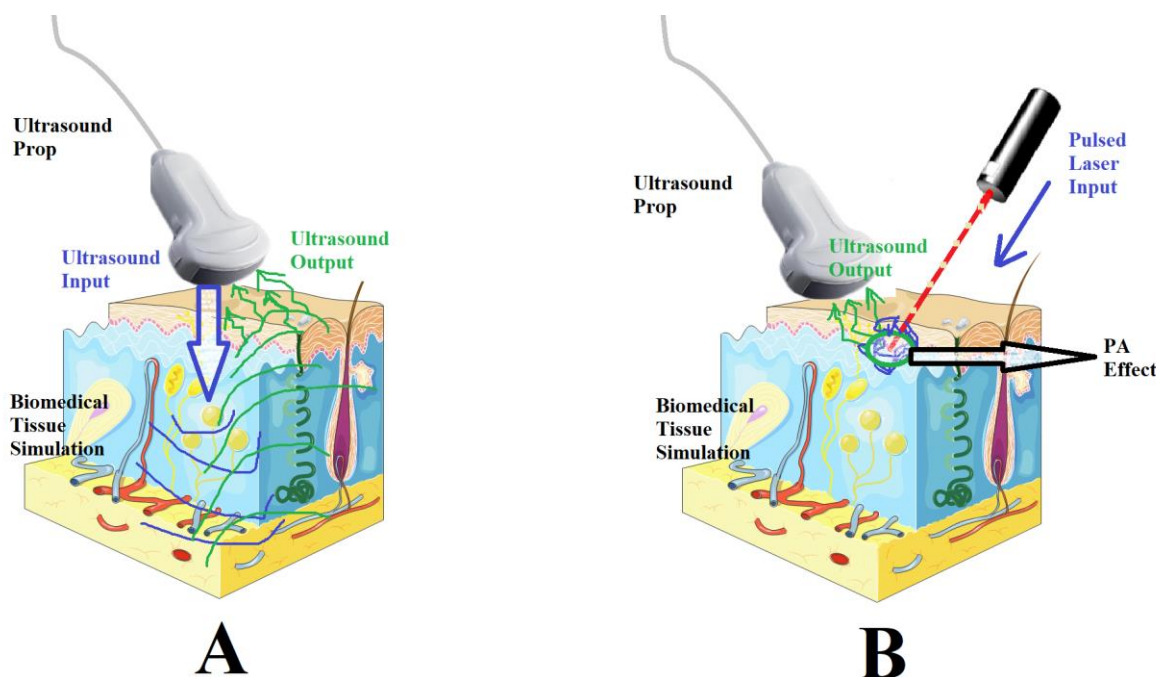


Fig. 6. A and B: simple illustration for the basic principle of ultrasound imaging and PAI, respectively. (The picture of the simulated skin tissue shown in the figure is taken from: <https://smart.servier.com>)

AUTHORS CONTRIBUTION

The following is authors' statement outlining their individual contributions to the paper using the relevant roles:

1. *Samir M. Badawy*: Supervision, Investigation, Conception and design of the work, Data analysis and interpretation, Methodology, Drafting the article, Critical revision of the article, and Final approval of the version to be published.
2. *Mohammed T. GadAllah*: Conception or design of the work, Data collection and tools, Data analysis and interpretation, Investigation, Methodology, Resources, Software, Drafting the article, Critical revision of the article, and Final approval of the version to be published.

3. *Abd El-Naser A. Mohamed, Alaa A. Hefnawy, Hassan E. Zidan, and Ghada M. El-Banby*: Supervision.

FUNDING STATEMENT:

The author received no financial support for the research, authorship and/ or publication of his article.

DECLARATION OF CONFLICTING INTERESTS STATEMENT:

The author declared no potential conflicts of interest with respect to the research, authorship or publication of his article.

REFERENCES

- [1.] Attia ABE, Balasundaram G, Moothanchery M, Dinish U S, Bi R, Ntziachristos V, Olivo M (Dec. 2019) A review of clinical photoacoustic imaging: Current and future trends. *Photoacoustics* 16(100144). <https://doi.org/10.1016/j.pacs.2019.100144>
- [2.] Beard P (2011) Biomedical photoacoustic imaging. *Interface Focus* (2011)1: 602–631. <https://doi.org/10.1098/rsfs.2011.0028>
- [3.] Wang LV (Jan./Feb. 2008) Tutorial on Photoacoustic Microscopy and Computed Tomography. *IEEE Journal of Selected Topics in Quantum Electronics* 14(1). <https://doi.org/10.1109/JSTQE.2007.913398>
- [4.] Bell AG (1880) On the production and reproduction of sound by light. *Amer. J. Sci.*, vol. 20, pp. 305–324. <https://doi.org/10.2475/ajs.s3-20.118.305>
- [5.] Bell AG (1881) LXVIII. Upon the production of sound by radiant energy. *The London, Edinburgh, and Dublin Philosophical Magazine and Journal of Science* 11 (71), pp. 510–528. <https://doi.org/10.1080/14786448108627053>
- [6.] Li J, Chen W, Yu B (2011) Recent Progress on Infrared Photoacoustic Spectroscopy Techniques. *Applied Spectroscopy Reviews* 46(6), 440–471. <https://doi.org/10.1080/05704928.2011.570835>
- [7.] Jones RW, McClelland J (2008) Fourier transform infrared photoacoustic spectroscopy of ageing composites. Ch. 6 in: “Ageing of composites”, edited by Rod Martin. Woodhead Publishing Ltd.
- [8.] Tian C, Chen S-L (2021) Recent developments in photoacoustic imaging and sensing for nondestructive testing and evaluation. *Visual Computing for Industry, Biomedicine, and Art*. <https://doi.org/10.1186/s42492-021-00073-1>
- [9.] Mikkonen T, Amiot C, Aalto A, Patokoski K, Genty G, Toivonen J (2019) Fourier Transform Photoacoustic Spectroscopy with Supercontinuum Light Source. 2019 Conference on Lasers and Electro-Optics Europe & European Quantum Electronics Conference (CLEO/Europe-EQEC). <https://doi.org/10.1109/CLEOE-EQEC.2019.8872426>
- [10.] Steinberg I, Huland DM, Vermesh O, Frostig HE, Tummers WS, Gambhir SS (June 2019) Photoacoustic clinical imaging. *Photoacoustics*, Vol. 14, pp. 77–98. <https://doi.org/10.1016/j.pacs.2019.05.001>
- [11.] Yang D-Y, Zhu Y, Kong J, Gong X, Xie Z, Mei W, Luo C, Du Z, Zhuang X, Liao X (2019) Light in and Sound Out: Review of Photoacoustic Imaging in Cardiovascular Medicine. *IEEE ACCESS*, Vol. 7. <http://dx.doi.org/10.1109/ACCESS.2019.2902543>
- [12.] Zackrisson S, Van-de-ven SMWY, Gambhir SS (2014) Light in and Sound Out: Emerging Translational Strategies for Photoacoustic Imaging. *Cancer Research* 74(4). <https://doi.org/10.1158/0008-5472.can-13-2387>
- [13.] Xia J, Wang LV (2013) Photoacoustic Tomography of the Brain. In: Madsen S. (eds) *Optical Methods and Instrumentation in Brain Imaging and Therapy*. Bioanalysis (Advanced Materials, Methods, and Devices), vol 3. Springer, New York, NY. https://doi.org/10.1007/978-1-4614-4978-2_6
- [14.] Hui J, Cheng J-X (2020) Intravascular Photoacoustic Imaging of Lipid-Laden Plaques: From Fundamental Concept Toward Clinical Translation. In: Zhou Q., Chen Z. (eds) *Multimodality Imaging*. Springer, Singapore. https://doi.org/10.1007/978-981-10-6307-7_4
- [15.] Li Y, Li L, Zhu L, Maslov K, Shi J, Hu P, Bo E, Yao J, Liang J, Wang L, Wang LV (2020) Snapshot photoacoustic topography through an ergodic relay for high-throughput imaging of optical absorption. *Nature Photonics*, 14, Pp. 164–170. <https://doi.org/10.1038/s41566-019-0576-2>
- [16.] Li L, Li Y, Zhang Y, Wang LV (May 2021) Snapshot photoacoustic topography through an ergodic relay of optical absorption in vivo. *Nature Protocols* (16): 2381–2394. <https://doi.org/10.1038/s41596-020-00487-w>
- [17.] Li Y, Li L, Zhu L, Shi J, Maslov K, Wang LV. (10 July 2020). Photoacoustic topography through an ergodic relay for functional imaging and biometric application in vivo. *Journal of Biomedical Optics*: 25(7), 070501. <https://doi.org/10.1117/1.JBO.25.7.070501>
- [18.] Yang J-M, Maslov K, Yang H-C, Zhou Q, Shung KK, Wang LV (2009) Photoacoustic endoscopy. *Optics Letters* 34(10): 1591–1593. <https://doi.org/10.1364/OL.34.001591>
- [19.] He Z, Wang P, Ye X (2021) Novel endoscopic optical diagnostic technologies in medical trial research: recent advancements and future prospects. *BioMed Eng OnLine* 20: 5. <https://doi.org/10.1186/s12938-020-00845-5>
- [20.] Bouy c C, Fauchaux M (Dec. 2017) Photoacoustic Imaging: Technology, Market and Trends: From research labs to clinical products. *Optik & Photonik*, 12 (5), pp. 20–21. <https://doi.org/10.1002/opph.201770507>
- [21.] Li y, Lu G, Zhou Q, Chen Z (2021) Advances in Endoscopic Photoacoustic Imaging. *Photonics* 2021, 8, 281. <https://doi.org/10.3390/photonics8070281>
- [22.] Wang LV, Gao L (2014) Photoacoustic microscopy and computed tomography: from bench to bedside. *Ann. Rev. Biomed. Eng.* 16. <https://doi.org/10.1146/annurev-bioeng-071813-104553>
- [23.] Yoon T-J, Cho Y-S (Nov. 2013) Recent advances in photoacoustic endoscopy. *World J Gastrointest Endosc* 5(11): 534–539. <http://dx.doi.org/10.4253/wjge.v5.i11.534>
- [24.] Yang J-M, Li C, Chen R, Zhou Q, Shung KK, Wang LV (June 2014) Catheter-based photoacoustic endoscope. *Journal of Biomedical Optics* 19(6), 066001. <http://dx.doi.org/10.1117/1.JBO.19.6.066001>
- [25.] Basij M, Karpiouk A, Winer I, Emelianov S, Mehrmohammadi M (Feb. 2021) Dual-Illumination Ultrasound/ Photoacoustic System for Cervical Cancer Imaging. *IEEE Photonics Journal* 13(1): 6900310. <https://doi.org/10.1109/JPHOT.2020.3043685>
- [26.] Ali Z, Zakian C, Ntziachristos V (2021) Ultra-broadband axicon transducer for optoacoustic endoscopy. *Scientific Reports* (2021)11: 1654. <https://doi.org/10.1038/s41598-021-81117-7>
- [27.] Wang B, Wang C, Zhong F, Pang W, Guo L, Peng K, Xiao J (Feb. 2021) 3D acoustic resolution-based photoacoustic endoscopy with dynamic focusing. *Quant Imaging Med Surg* 11(2): 685–696. <https://doi.org/10.21037/QIMS-20-625>
- [28.] Yang J-M, Favazza C, Yao J, Chen R, Zhou Q, Shung KK, Wang LV (April 2015) Three-Dimensional Photoacoustic Endoscopic Imaging of the Rabbit Esophagus. *PLoS ONE* 10(4): e0120269. <https://doi.org/10.1371/journal.pone.0120269>
- [29.] Wang LV, Beare GK (2013) Photoacoustic Tomography: Ultrasonically Breaking through the Optical Diffusion and Diffraction Limits. 2013 Conference on Lasers & Electro-Optics Europe & International Quantum Electronics Conference CLEO EUROPE/IQEC. Munich, Germany. <https://doi.org/10.1109/CLEOE-IQEC.2013.6801491>
- [30.] Wang LV (2009) Photoacoustic Tomography: High-Resolution Imaging of Optical Contrast in Vivo at Superdepths. 2009 IEEE International Symposium on Biomedical Imaging: From Nano to Macro. Boston, MA, USA. <https://doi.org/10.1109/ISBI.2009.5193275>
- [31.] Wang LV, Yao J (2016) A practical guide to photoacoustic tomography in the life sciences. *Nature Methods*, 13(8): 627–638. <https://doi.org/10.1038/nmeth.3925>
- [32.] Yao J, Wang LV (June 2021) Perspective on fast-evolving photoacoustic tomography. *Journal of Biomedical Optics* 26(6): 060602. <https://doi.org/10.1117/1.JBO.26.6.060602>
- [33.] Wang LV, Song Hu S (2012) Photoacoustic Tomography: In Vivo Imaging from Organelles to Organs. *Science* 335(6075): pp. 1458–1462. <https://doi.org/10.1126/science.1216210>
- [34.] Yao J, Wang LV (2011) Photoacoustic tomography: fundamentals, advances and prospects. *Contrast Media Mol. Imaging* 6(5):332–45. <https://doi.org/10.1002/cmml.443>
- [35.] Wang LV (Dec. 2008) Prospects of photoacoustic tomography. *Medical Physics* 35(12): 5758–5767. <https://doi.org/10.1118/1.3013698>
- [36.] Xia J, Wang LV (May 2014) Small-animal whole-body photoacoustic tomography: a review. *IEEE - TBME* 61(5). <https://doi.org/10.1109/tbme.2013.2283507>
- [37.] Xu W, Leskinen J, Tick J, Happonen E, Tarvainen T, Lehto V-P (2020) Black mesoporous silicon as contrast agent for LED-based 3D photoacoustic tomography. *ACS Appl. Mater. Interf.*, 12(5): 5456–5461. <https://doi.org/10.1021/acsami.9b18844>
- [38.] Pitner JB, Rajamahendiran RM, Thomas RD (Jan. 9, 2020) Hydrophorphyris for photoacoustic imaging. United States patent application. Appl. No.: 16/483394. Pub. No.: US 2020/0009272 A1.
- [39.] Nasirivanani M, Xia J, Wan H, Bauer AQ, Culver JP, Wang LV (Jan. 7, 2014) High-resolution photoacoustic tomography of resting-state functional connectivity in the mouse brain. *PNAS* 111(1): 21–26. <https://doi.org/10.1073/pnas.1311868111>
- [40.] Razansky D, Distel M, Vinegoni C, Ma R, Perrimon N, Koster RW, Ntziachristos V (July 2009) Multispectral opto-acoustic tomography of deep-seated fluorescent proteins in vivo. *Nature Photonics* 3: 412–417. <https://doi.org/10.1038/nphoton.2009.98>
- [41.] Razansky D, Vinegoni C, Ntziachristos V (2007) Multispectral photoacoustic imaging of fluorochromes in small animals. *Optics Letters* 32(19): 2891–2893. <https://doi.org/10.1364/OL.32.002891>
- [42.] Ma R, Taruttis A, Ntziachristos V, Razansky D (2009) Multispectral optoacoustic tomography (MSOT) scanner for whole-body small animal imaging. *Optics Express*, 17(24). <https://doi.org/10.1364/oe.17.021414>
- [43.] Razansky D, Buehler A, Ntziachristos V (2011) Volumetric real-time multispectral photoacoustic tomography of biomarkers. *Nature Protocols* 6(8). <https://doi.org/10.1038/nprot.2011.351>

- [44.] Taruttis A, Morscher S, Burton NC, Razansky D, Ntziachristos V (Jan. 2012) Fast Multispectral Optoacoustic Tomography (MSOT) for Dynamic Imaging of Pharmacokinetics and Biodistribution in Multiple Organs. *Plos One* 7(1): e30491. <https://doi.org/10.1371/journal.pone.0030491>
- [45.] Morscher S, Driessen WHP, Claussen J, Burton NC (2014) Semi-quantitative Multispectral Optoacoustic Tomography (MSOT) for volumetric PK imaging of gastric emptying. *Photoacoustics*, 2(3): 103–110. <https://doi.org/10.1016/j.pacs.2014.06.001>
- [46.] Taruttis A, van Dam GM, Ntziachristos V (2015) Mesoscopic and Macroscopic Optoacoustic Imaging of Cancer. *Cancer Res* 75(8). <https://doi.org/10.1158/0008-5472.can-14-2522>
- [47.] Neuschmelting V, Burton NC, Lockau H, Ulrich A, Harmsen S, Ntziachristos V, Kircher MF (2016) Performance of a Multispectral Optoacoustic Tomography (MSOT) System equipped with 2D vs. 3D Handheld Probes for Potential Clinical Translation. *Photoacoustics*, 4 (1): 1-10. <https://doi.org/10.1016/j.pacs.2015.12.001>
- [48.] Chuah SY, Attia ABE, Long V, Ho CJH, Malempati P, Fu CY, Ford SJ, Lee JSS, Tan WP, Razansky D, Olivo M, Thng S (2017) Structural and functional 3D mapping of skin tumours with non-invasive multispectral optoacoustic tomography. *Skin Research and Technology* 23(2): 221–226. <https://doi.org/10.1111/srt.12326>
- [49.] Diot G, Metz S, Noske A, Liapis E, Schroeder B, Ovsepian SV, Meier R, Rummey E, Ntziachristos V (2017) Multispectral Optoacoustic Tomography (MSOT) of Human Breast Cancer. *Clin Cancer Res* 23(22):6912-6922. <https://doi.org/10.1158/1078-0432.ccr-16-3200>
- [50.] Cong Z, Yang F, Cao L, Wen H, Fu T, Ma S, Liu C, Quan L, Liao Y (2018) Multispectral optoacoustic tomography (MSOT) for imaging the particle size-dependent intratumoral distribution of polymeric micelles. *International Journal of Nanomedicine* 13: 8549-8560. <https://doi.org/10.2147/ijn.s185726>
- [51.] Roll W, Markwardt NA, Masthoff M, Helfen A, Claussen J, Eisenblätter M, Hasenbach A, Hermann S, Karlas A, Wildgruber M, Ntziachristos V, Schäfers M (2019) Multispectral Optoacoustic Tomography of Benign and Malignant Thyroid Disorders: A Pilot Study. *J Nucl Med* 60(10):1461-1466. <https://doi.org/10.2967/jnumed.118.222174>
- [52.] Huang Y, Qi Y, Zhan C, Zeng F, Wu S (2019) Diagnosing Drug-Induced Liver Injury by Multispectral Optoacoustic Tomography and Fluorescence Imaging Using a Leucine-Aminopeptidase-Activated Probe. *Anal Chem* 91(13): 8085–8092. <https://doi.org/10.1021/acs.analchem.9b00107>
- [53.] Olefir I, Ghazaryan A, Yang H, Malekzadeh-Najafabadi J, Glasl S, Symvoulidis P, O'Leary VB, Sergiadis G, Ntziachristos V, Ovsepian SV (2019) Spatial and Spectral Mapping and Decomposition of Neural Dynamics and Organization of the Mouse Brain with Multispectral Optoacoustic Tomography. *Cell Rep* 26(10):2833-2846.e3. <https://doi.org/10.1016/j.celrep.2019.02.020>
- [54.] Bhutiani N, Samykutty A, McMasters KM, Egilmez NK, McNally LR (2019) In vivo tracking of orally-administered particles within the gastrointestinal tract of murine models using multispectral optoacoustic tomography. *Photoacoustics*, 13: 46–52. <https://dx.doi.org/10.1016%2Fj.pacs.2018.11.003>
- [55.] Anani T, Brannen A, Panizzi P, Duin EC, David AE (2020) Quantitative, real-time in vivo tracking of magnetic nanoparticles using multispectral optoacoustic tomography (MSOT) imaging. *J. of Pharm. and Biomed. Analysis* 178: 112951. <https://doi.org/10.1016/j.jpba.2019.112951>
- [56.] Gehrung M, Tomaszewski M, McIntyre D, Disselhorst J, Bohndiek S (2020) Co-Registration of Optoacoustic Tomography and Magnetic Resonance Imaging Data from Murine Tumour Models. *Photoacoustics* 18: 100147. <https://dx.doi.org/10.1016%2Fj.pacs.2019.100147>
- [57.] Wang LV (2009) Photoacoustic Tomography: High-Resolution Imaging of Optical Contrast in Vivo at New Depths. 2009 IEEE LEOS Annual Meeting Conference Proceedings, Belek-Antalya, Turkey. <https://doi.org/10.1109/LEOS.2009.5343227>
- [58.] Maslov K, Stoica G, Wang LV (2005) In vivo dark-field reflection-mode photoacoustic microscopy. *Optics Letters* 30(6): 625-627. <https://doi.org/10.1364/OL.30.000625>
- [59.] Yao J, Wang LV (2013) Photoacoustic microscopy. *Laser & Photonics Reviews* 7(5): 758-778. <https://doi.org/10.1002/lpor.201200060>
- [60.] Omar M, Aguirre J, Ntziachristos V (2019) Optoacoustic mesoscopy for biomedicine. *Nat Biomed Eng* 3(5):354-370. <https://doi.org/10.1038/s41551-019-0377-4>
- [61.] Ntziachristos V (2010) Going deeper than microscopy: the optical imaging frontier in biology. *Nature Methods* 7(8): 603-614. <https://doi.org/10.1038/nmeth.1483>
- [62.] Schwarz M, Omar M, Buehler A, Aguirre J, Ntziachristos V (2015) Implications of Ultrasound Frequency in Optoacoustic Mesoscopy of the Skin. *IEEE Trans Med Imaging* 34(2). <https://doi.org/10.1109/TMI.2014.2365239>
- [63.] Omar M, Gateau J, Ntziachristos V (2013) Raster-scan optoacoustic mesoscopy in the 25–125 MHz range. *Optics Letters* 38(14). <https://doi.org/10.1364/ol.38.002472>
- [64.] Omar M, Soliman D, Gateau J, Ntziachristos V (2014) Ultrawideband reflection-mode optoacoustic mesoscopy. *Optics Letters*, 39(13). <https://doi.org/10.1364/ol.39.003911>
- [65.] Omar M, Schwarz M, Soliman D, Symvoulidis P, Ntziachristos V (Feb. 2015) Pushing the Optical Imaging Limits of Cancer with Multi-Frequency-Band Raster-Scan Optoacoustic Mesoscopy (RSOM). *Neoplasia* 17(2): 208–214. <https://doi.org/10.1016/j.neo.2014.12.010>
- [66.] Aguirre J, Schwarz M, Garzorz N, Omar M, Buehler A, Eyerich K, Ntziachristos V (2017) Precision assessment of label-free psoriasis biomarkers with ultra-broadband optoacoustic mesoscopy. *Nature Biomedical Engineering*. 1(0068). <https://doi.org/10.1038/s41551-017-0068>
- [67.] Bereznoi A, Schwarz M, Buehler A, Ovsepian S V, Aguirre J, Ntziachristos V (2018) Assessing hyperthermia-induced vasodilation in human skin in vivo using optoacoustic mesoscopy. *J Biophotonics* (11)11: e201700359. <https://doi.org/10.1002/jbio.201700359>
- [68.] Aguirre J, Hindelang B, Bereznoia A, Darsowb U, Laufferb F, Eyerichb K, Biedermannb T, Ntziachristosa V (2018) Assessing nailfold microvascular structure with ultra-wideband raster-scan optoacoustic mesoscopy. *Photoacoustics*, 10 (2018): 31–37. <https://doi.org/10.1016/j.pacs.2018.02.002>
- [69.] Knieling F, et al (2018) Raster-Scanning Optoacoustic Mesoscopy for Gastrointestinal Imaging at High Resolution. *Gastroenterology* 154(4): 807–809.e3. <https://doi.org/10.1053/j.gastro.2017.11.285>
- [70.] Dangi A, Agrawal S, Datta GR, Srinivasan V, Kothapalli S-R (2020) Towards a Low-Cost and Portable Photoacoustic Microscope for Point-of-Care and Wearable Applications. *IEEE Sensors Journal*, 20(13): 6881-6888. <https://doi.org/10.1109/jsen.2019.2935684>
- [71.] Li X, Tsang VTC, Kang L, Zhang Y, Wong TTW (Jan 2021) High-speed high-resolution laser diode-based photoacoustic microscopy for in vivo microvasculature imaging. *Vis. Comput. Ind. Biomed. Art* 4, 1 (2021). <https://doi.org/10.1186/s42492-020-00067-5>
- [72.] Singh MS, Thomas A (2019) Photoacoustic elastography imaging: a review. *Journal of Biomedical Optics* 24(4). <https://doi.org/10.1117/1.jbo.24.4.040902>
- [73.] Hai P, Yao J, Li G, Li C, Wang L V (2016) Photoacoustic elastography. *Opt. Lett.* 41(4): 725–728. <https://doi.org/10.1364/OL.41.000725>
- [74.] Gao G, Yang S, Xing D (2011) Viscoelasticity imaging of biological tissues with phase-resolved photoacoustic measurement. *Opt. Lett.* 36(17). <https://doi.org/10.1364/OL.36.003341>
- [75.] Parker KJ, Doyley MM, Rubens DJ (2011) Imaging the elastic properties of tissue: the 20-year perspective. *Phys Med Biol* 56(1). <https://doi.org/10.1088/0031-9155/56/1/R01>
- [76.] Hai P, Zhou Y, Liang J, Li C, Wang LV (2015) Photoacoustic tomography of vascular compliance in humans. *Journal of Biomedical Optics* 20(12): 126008. <https://doi.org/10.1117/1.jbo.20.12.126008>
- [77.] Hai P, Zhou Y, Gong L, Wang LV (2016) Quantitative photoacoustic elastography in humans. *Journal of Biomedical Optics* 21(6): 066011. <https://doi.org/10.1117/1.JBO.21.6.066011>
- [78.] Hai P, Zhou Y, Gong L, Wang LV (2017) Quantitative photoacoustic elastography of Young's modulus in humans. *Proc. SPIE 10064, Photons Plus Ultrasound: Imaging and Sensing 2017*, 100640B. <https://doi.org/10.1117/12.2252790>
- [79.] Monchalin J-P (1986) Optical Detection of Ultrasound, *IEEE Transactions on Ultrasonics, Ferroelectrics, and Frequency Control* 33(5): 485-499. <https://doi.org/10.1109/T-UFFC.1986.26860>
- [80.] Dong B, Sun C, Zhang HF (2017) Optical Detection of Ultrasound in Photoacoustic Imaging. *IEEE Transactions on Biomedical Engineering* 64(1): 4-15. <https://doi.org/10.1109/TBME.2016.2605451>
- [81.] Zhang X, Fincke JR, Wynn CM, Johnson MR, Haupt RW, Anthony BW (2019) Full noncontact laser ultrasound: first human data. *Light: Science & Applications* 8:119. <https://doi.org/10.1038/s41377-019-0229-8>

- [82.] Maiman TH (1960) Stimulated Optical Radiation. *Nature* 187: 493-494. <https://doi.org/10.1038/187493a0>
- [83.] Monchalain J-P (2004) Laser-ultrasonics: from the laboratory to industry. AIP Conference Proceedings 700, 3 (2004). <https://doi.org/10.1063/1.1711602>
- [84.] Rousseau G, Blouin A, Monchalain J-P (2012) Non-contact photoacoustic tomography and ultrasonography for tissue imaging. *Biomed Opt Express* 3(1): 16-25. <https://doi.org/10.1364/BOE.3.000016>
- [85.] Rousseau G, Gauthier B, Blouin A, Monchalain J-P (2012) Non-contact biomedical photoacoustic and ultrasound imaging. *Journal of Biomedical Optics* 17(6): 061217. <https://doi.org/10.1117/1.JBO.17.6.061217>
- [86.] Haupt R (2017) Non-Contact Laser Ultrasound for Medical Imaging. 2017 IEEE International Ultrasonics Symposium (IUS), Washington, DC, USA. <https://doi.org/10.1109/ULTSYM.2017.8091525>
- [87.] Haupt R, Wynn C, Anthony B, Fincke J, Samir A, Zhang X (2017) Non-Contact Laser Ultrasound Concept for Biomedical Imaging. 2017 IEEE International Ultrasonics Symposium (IUS), Washington, DC, USA. <https://doi.org/10.1109/ULTSYM.2017.8091941>
- [88.] Johnson JL, Shragge J, van Wijk K (2017) Nonconfocal all-optical laserultrasound and photoacoustic imaging system for angle-dependent deep tissue imaging. *J Biomed Opt* 22(4): 041014. <https://doi.org/10.1117/1.JBO.22.4.041014>
- [89.] Johnson JL, Merrilees M, Shragge J, van Wijk K (2018) All-optical extravascular laser-ultrasound and photoacoustic imaging of calcified atherosclerotic plaque in excised carotid artery. *Photoacoustics* 9: 62–72. <https://doi.org/10.1016/j.pacs.2018.01.002>
- [90.] Haupt R, Zhang X, Fincke J, Richardson J, Hughes J, Anthony B, Samir A (2019) Non-Contact laser ultrasound (N-CLUS) system for medical imaging and elastography. 2019 IEEE International Ultrasonics Symposium (IUS), Glasgow, UK. <https://doi.org/10.1109/ULTSYM.2019.8925569>
- [91.] Siegel RL, Miller KD, Jemal A (2020) Cancer Statistics. *CA Cancer J. Clin.*, 70(1), pp. 7–30, Jan./Feb. 2020. <https://doi.org/10.3322/caac.21590>
- [92.] American Cancer Society (ACS) (2020) Cancer Facts & Figures 2020, Atlanta: ACS.
- [93.] International Agency for Research on Cancer (2014) World Cancer Report 2014, edited by Stewart BW and Wild CP, WHO, Lyon 2014.
- [94.] Chen Y-S, Yeager D, Emelianov SY (2014) Photoacoustic Imaging for Cancer Diagnosis and Therapy Guidance. Ch. 9 (pp. 139-158) in: *Cancer Theranostics*, edited by: Chen X and Wong S. Academic Press. <https://doi.org/10.1016/B978-0-12-407722-5.00009-8>
- [95.] Gargiulo S, Albanese S, Mancini M (2019) State-of-the-Art Preclinical Photoacoustic Imaging in Oncology: Recent Advances in Cancer Theranostics. *Contrast Media & Molecular Imaging* (2019)5080267. <https://doi.org/10.1155/2019/5080267>
- [96.] American Cancer Society (ACS), Breast Cancer Facts & Figures 2019-2020, Atlanta: ACS, Inc. 2019. URL (Last seen in 30th Aug. 2021): <https://www.cancer.org/content/dam/cancer-org/research/cancer-facts-and-statistics/breast-cancer-facts-and-figures/breast-cancer-facts-and-figures-2019-2020.pdf>
- [97.] Badawy SM, Hefnawy AA, Zidan HE, GadAllah MT (2017) Breast Cancer Detection with Mammogram Segmentation: A Qualitative Study. *IJACSA* 8(10). <https://dx.doi.org/10.14569/IJACSA.2017.081016>
- [98.] Badawy SM, Mohamed AA, Hefnawy AA, Zidan HE, GadAllah MT, Banby GM (May 2021) Automatic semantic segmentation of breast tumors in ultrasound images based on combining fuzzy logic and deep learning—A feasibility study. *PLoS ONE* 16(5): e0251899. <https://doi.org/10.1371/journal.pone.0251899>
- [99.] Shan C, Tan T, Han J, Huang D (2021) Ultrasound tissue classification: a review. *Artificial Intelligence Review* (2021) 54:3055–3088. <https://doi.org/10.1007/s10462-020-09920-8>
- [100.] Badawy SM, Zidan HE, Mohamed AA, Hefnawy AA, GadAllah MT, El-Banby GM (July 2021) A Wavelet - Fuzzy Combination Based Approach for Efficient Cancer Characterization in Breast Ultrasound Images. 2021 International Conference on Electronic Engineering (ICEEM), Menouf, Menoufia, Egypt. <https://doi.org/10.1109/ICEEM52022.2021.9480631>
- [101.] Badawy SM, Mohamed AA, Hefnawy AA, Zidan HE, GadAllah MT, El-Banby GM (July 2021) Classification of Breast Ultrasound Images Based on Convolutional Neural Networks – A Comparative Study. 2021 International Telecommunications Conference (ITC-Egypt), Alexandria, Egypt. <https://doi.org/10.1109/ITC-Egypt52936.2021.9513972>
- [102.] Kuhl C (Aug. 2007) The Current Status of Breast MR Imaging - Part I. Choice of Technique, Image Interpretation, Diagnostic Accuracy, and Transfer to Clinical Practice. *Radiology* 244(2). <https://doi.org/10.1148/radiol.2442051620>
- [103.] Kuhl C (Sept. 2007) Current Status of Breast MR Imaging Part 2. Clinical Applications. *Radiology* 244(3). <https://doi.org/10.1148/radiol.2443051661>
- [104.] Manohar S, Dantuma M (2019) Current and future trends in photoacoustic breast imaging. *Photoacoustics* 16: 100134. <https://doi.org/10.1016/j.pacs.2019.04.004>
- [105.] Nyayapathi N, Xia J (Dec. 2019) Photoacoustic imaging of breast cancer: a mini review of system design and image features. *Journal of Biomedical Optics* 24(12): 121911. <https://doi.org/10.1117/1.JBO.24.12.121911>
- [106.] Manohar S, Kharine A, van-Hespen JCG, Steenbergen W, van-Leeuwen TG (2005) The Twente Photoacoustic Mammoscope: system overview and performance. *Phys. Med. Biol.* 50 (11): 2543–2557. <https://doi.org/10.1088/0031-9155/50/11/007>
- [107.] Piras D, Xia W, Heijblom M, Ten-Tije EM, Van-Hespen J, Steenbergen W, Van-Leeuwen TG, Manohar S, Van-den-Eng F, Klaase JM (2011) Breast imaging with the Twente Photoacoustic Mammoscope. 2011 International Workshop on Biophotonics. Parma, Italy. <https://doi.org/10.1109/IWBP.2011.5954818>
- [108.] Lin L, Hu P, Shi J, Appleton CM, Maslov K, Li L, Zhang R, Wang LV (2018) Single-breath-hold photoacoustic computed tomography of the breast. *Nature Communications* 9: 2352. <https://doi.org/10.1038/s41467-018-04576-z>
- [109.] Shiina T, Toi M, Yagi T (2018) Development and clinical translation of photoacoustic mammography. *Biomedical Engineering Letters* 8: 157–165. <https://doi.org/10.1007/s13534-018-0070-7>
- [110.] Rao AP, Bokde N, Sinha S (2020) Photoacoustic Imaging for Management of Breast Cancer: A Literature Review and Future Perspectives. *Appl. Sci.* 10(3): 767. <https://doi.org/10.3390/app10030767>
- [111.] Lin L, Hu P, Tong X, Na S, Cao R, Yuan X, Garrett DC, Shi J, Maslov K, Wang LV (2021) High-speed three-dimensional photoacoustic computed tomography for preclinical research and clinical translation. *Nature Communications* 12: 882. <https://doi.org/10.1038/s41467-021-21232-1>
- [112.] American Thyroid Association (ATA) (2016) Thyroid Cancer, (Papillary and Follicular), ATA. URL (Last seen in 30th Aug. 2021): https://www.thyroid.org/wp-content/uploads/patients/brochures/ThyroidCancer_brochure.pdf
- [113.] Kang J, Chung WY, Kang S-W, Kwon HJ, Yoo J, Kim E-K, Chang JH, Song T-K, Lee S, Kwak JY (2014) Ex Vivo Estimation of Photoacoustic Imaging for Detecting Thyroid Microcalcifications. *PLoS One* 9(11): e113358. <https://doi.org/10.1371/journal.pone.0113358>
- [114.] Dogra VS, Chinni BK, Valluru KS, Moalem J, Giampoli EJ, Evans K, Rao NA (2014) Preliminary Results of Ex Vivo Multispectral Photoacoustic Imaging in the Management of Thyroid Cancer. *AJR* 202(6): W552-W558. <https://doi.org/10.2214/ajr.13.11433>
- [115.] Dima A, Ntziachristos V (2016) In-vivo handheld optoacoustic tomography of the human thyroid. *Photoacoustics* 4(2): 65–69. <https://doi.org/10.1016/j.pacs.2016.05.003>
- [116.] Rao B, Leng X, Zeng Y, Lin Y, Chen R, Zhou Q, Hagemann AR, Kuroki LM, McCourt CK, Mutch DG, Powell MA, Hagemann IS, Zhu Q (2019) Optical Resolution Photoacoustic Microscopy of Ovary and Fallopian Tube. *Scientific Reports* 9:14306. <https://doi.org/10.1038/s41598-019-50743-7>
- [117.] Nandy S, Mostafa A, Hagemann IS, Powell MA, Amidi E, Robinson K, Mutch DG, Siegel C, Zhu Q (2018) Evaluation of Ovarian Cancer: Initial Application of Coregistered Photoacoustic Tomography and US. *Radiology* 289(3):740-747. <https://doi.org/10.1148/radiol.2018180666>
- [118.] Amidi E, Yang G, Shihab Uddin KM, Luo H, Middleton W, Powell M, Siegel C, Zhu Q (2021) Role of blood oxygenation saturation in ovarian cancer diagnosis using multi-spectral photoacoustic tomography. *Journal of Biophotonics*. (2021)14: e202000368. <https://doi.org/10.1002/jbio.202000368>
- [119.] Salehi HS, Li H, Merkulov A, Kumavor PD, Vavadi H, Sanders M, Kueck A, Brewer MA, Zhu Q (2016) Coregistered photoacoustic and ultrasound imaging and classification of ovarian cancer: ex vivo and in vivo studies. *J of Biomedical Optics* 21(4): 046006. <https://doi.org/10.1117/1.jbo.21.4.046006>
- [120.] Kothapalli S-R et al (Aug. 2019) Simultaneous transrectal ultrasound and photoacoustic human prostate imaging. *Science Translational Medicine* 11(507): eaav2169. <https://doi.org/10.1126/scitranslmed.aav2169>
- [121.] Dogra VS, Chinni BK, Valluru KS, Joseph JV, Ghazi A, Yao JL, Evans K, Messing EM, Rao NA (2013) Multispectral Photoacoustic Imaging of Prostate Cancer: Preliminary Ex-vivo Results. *Journal of Clinical Imaging Science* 3(41). <https://doi.org/10.4103/2156-7514.119139>
- [122.] Bungart BL, Lan L, Wang P, Li R, Koche MO, Cheng L, Masterson TA, Dundar M, Cheng J-X (2018) Photoacoustic tomography of intact human prostates and vascular texture analysis identify prostate cancer biopsy

- targets. Photoacoustics 11: 46–55. <https://doi.org/10.1016/j.pacs.2018.07.006>
- [123.]Moradi H, Tang S, Salcudean SE (2019) Towards Intra-operative Prostate Photoacoustic Imaging: Configuration Evaluation and Implementation Using the da Vinci Research Kit. IEEE TMI 38(1): 57–68. <https://doi.org/10.1109/TMI.2018.2855166>
- [124.]Zhang H, Huang S, Chen Y, Xie W, Zhang M, Pan J, Sato N, Wang X, Wu D, Cheng Q (2020) Examining the technical feasibility of prostate cancer molecular imaging by transrectal photoacoustic tomography with transurethral illumination. Exp Biol Med (Maywood) 245(4): 313–320. <https://doi.org/10.1177/1535370219884356>
- [125.]Ai M, Youn J-I, Salcudean SE, Rohling R, Abolmaesumi P, Tang S (2019) Photoacoustic tomography for imaging the prostate: a transurethral illumination probe design and application. Biomedical Optics Express 10(5): 2588–2605. <https://doi.org/10.1364/boe.10.002588>
- [126.]Saalberg Y, Bruhns H, Wolff M (2017) Photoacoustic Spectroscopy for the Determination of Lung Cancer Biomarkers—A Preliminary Investigation. Sensors 17(1): 210. <https://doi.org/10.3390/s17010210>
- [127.]Gargiulo S, Albanese S, Mancini M (2019) State-of-the-Art Preclinical Photoacoustic Imaging in Oncology: Recent Advances in Cancer Theranostics. Contrast Media & Molecular Imaging 2019(5080267). <https://doi.org/10.1155/2019/5080267>
- [128.]Raes F, Sobilo J, Le-Mée M, Rétif S, Natkunarajah S, Lerondel S, Le-Pape A (2016) High Resolution Ultrasound and Photoacoustic Imaging of Orthotopic Lung Cancer in Mice: New Perspectives for Onco-Pharmacology. PLOS One 11(4): e0153532. <https://doi.org/10.1371/journal.pone.0153532>
- [129.]Jung H, Park S, Gunasekaran GR, Jeon M, Cho Y-E, Baek M-C, Park JY, Shim G, Oh Y-K, Kim I-S, Kim C, Lee B (2019) A peptide probe enables photoacoustic-guided imaging and drug delivery to lung tumors in K-rasLA2 mutant mice. Cancer Res 79(16): 4271–4282. <https://doi.org/10.1158/0008-5472.can-18-3089>
- [130.]Jose J, Grootendorst DJ, Vijn TW, Wouters M, van-Boven H, van-Leeuwen TG, Steenbergen W, Ruers TJM, Manohar S (2011) Initial results of imaging melanoma metastasis in resected human lymph nodes using photoacoustic computed tomography. Journal of Biomedical Optics 16(9): 096021. <https://doi.org/10.1117/1.3631705>
- [131.]Zabihian B, Weingast J, Liu M, Zhang E, Beard P, Pehamberger H, Drexler W, Hermann B (2015) In vivo dual-modality photoacoustic and optical coherence tomography imaging of human dermatological pathologies. Biomedical Optics Express 6(9): 3163–3178. <https://doi.org/10.1364/boe.6.003163>
- [132.]Zeitouni NC, Rohrbach DJ, Aksahin M, Sunar U (April 2015) Preoperative Ultrasound and Photoacoustic Imaging of Nonmelanoma Skin Cancers. Dermatologic Surgery, Letters and Communications 41(4): 525–528. <https://doi.org/10.1097/dss.0000000000000317>
- [133.]Zhou Y, Tripathi SV, Rosman I, Ma J, Hai P, Linette GP, Council ML, Fields RC, Wang LV, Cornelius LA (2017) Noninvasive Determination of Melanoma Depth using a Handheld Photoacoustic Probe. Journal of Investigative Dermatology 137(6): 1370–1372. <https://doi.org/10.1016/j.jid.2017.01.016>
- [134.]Attia ABE, Chuah SY, Razansky D, Ho CJH, Malempati P, Dinish US, Bi R, Fu CY, Ford SJ, Lee JS, Tan MWP, Olivo M, Thng STG (2017) Noninvasive real-time characterization of non-melanoma skin cancers with handheld optoacoustic probes. Photoacoustics 7 (2017): 20–26. <https://doi.org/10.1016/j.pacs.2017.05.003>
- [135.]Kratkiewicz K, Manwar R, Rajabi-Estarabadi A, Fakhoury J, Meiliute J, Daveluy S, Mehregan D, Avanaki KM (2019) Photoacoustic/Ultrasound/Optical Coherence Tomography Evaluation of Melanoma Lesion and Healthy Skin in a Swine Model. Sensors 19(12): 2815. <https://doi.org/10.3390/s19122815>
- [136.]Raghu P (2019) Out of breath: molecular description of cellular responses to hypoxia – 2019 Nobel Prize for Physiology or Medicine. Current Science 117(9): 1418–1419. URL (Last seen in 30th Aug. 2021): <https://www.currentscience.ac.in/Volumes/117/09/1418.pdf>
- [137.]Jr WGK, Ratcliffe PJ, Semenza GL (2016) Pathways for Oxygen Regulation and Homeostasis: The 2016 Albert Lasker Basic Medical Research Award. (View Point) JAMA 316(12): 1252–1253. <https://doi.org/10.1001/jama.2016.12386>
- [138.]Marino PL (2007) Oxygen and Carbon Dioxide Transport; Ch.2. and Oximetry and Capnography; Ch. 20. in: The ICU Book, 3rd Edition (2007), ISBN: 13: 9 78-0-07817-4802-5. Lippincott Williams & Wilkins.
- [139.]Khaw K, Schultz SM, Mohammed M, Chen Z, Ashi K, Sehgal CM (2018) Photoacoustic imaging for assessing flow-mediated oxygenation for peripheral arterial disease. 2018 IEEE International Ultrasonics Symposium (IUS), Kobe, Japan. <https://doi.org/10.1109/ULTSYM.2018.8580057>
- [140.]Li M, Tang Y, Yao J (2018) Photoacoustic tomography of blood oxygenation: A mini review. Photoacoustics 10 (2018): 65–73. <https://doi.org/10.1016/j.pacs.2018.05.001>
- [141.]Zhang HF, Maslov K, Wang LV (2009) Dark-Field Confocal Photoacoustic Microscopy. Ch. 21 in: Photoacoustic imaging and Spectroscopy, edited by Wang LV, Taylor & Francis Group, LLC. <https://doi.org/10.1201/9781420059922>
- [142.]Needles A, Heimiller A, Ephrat P, Bilan-Tracey C, Trujillo A, Theodoropoulos C, Hirson D, Foster FS (2010) Development of a Combined Photoacoustic Micro-Ultrasound System for Estimating Blood Oxygenation. 2010 IEEE International Ultrasonics Symposium, San Diego, CA, USA. <https://doi.org/10.1109/ULTSYM.2010.5935920>
- [143.]Gerling M, Zhao Y, Nania S, Norberg KJ, Verbeke CS, Englert B, Kuiper RV, Bergström A, Hassan M, Neesse A, Löhr JM, Heuchel RL (2014) Real-time assessment of tissue hypoxia in vivo with combined photoacoustics and high-frequency ultrasound. Theranostics 4(6): 604–613. <https://doi.org/10.7150/thno.7996>
- [144.]Yao J, Maslov KI, Shi Y, Taber LA, Wang LV (2010) In vivo photoacoustic imaging of transverse blood flow by using Doppler broadening of bandwidth. Opt Lett 35(9): 1419–1421. <https://doi.org/10.1364/OL.35.001419>
- [145.]Van den Berg PJ, Daoudi K, Steenbergen W (2015) Review of photoacoustic flow imaging: its current state and its promises. Photoacoustics 3(3): 89–99. <https://doi.org/10.1016/j.pacs.2015.08.001>
- [146.]Liu Y, Nie L, Chen X (2016) Photoacoustic Molecular Imaging: From Multiscale Biomedical Applications Towards Early-Stage Theranostics. Trends in Biotechnology 34(5): 420–433. <https://doi.org/10.1016/j.tibtech.2016.02.001>
- [147.]Yao J, Wang LV (2014) Photoacoustic brain imaging: from microscopic to macroscopic scales. Neurophotonics 1(1): 011003. <https://doi.org/10.1117/1.nph.1.1.011003>
- [148.]Park SJ, Ho CJH, Arai S, Samanta A, Olivo M, Chang YT (2019) Visualizing Alzheimer's Disease Mouse Brain with Multispectral Optoacoustic Tomography using a Fluorescent probe, CDnr7. Scientific Reports 9(1):12052. <https://doi.org/10.1038/s41598-019-48329-4>
- [149.]Yang X, Wang LV (2008) Monkey brain cortex imaging by photoacoustic tomography. Journal of Biomedical Optics 13(4): 044009. <https://doi.org/10.1117/1.2967907>
- [150.]Lou Y, Xia J, Wang LV (2014) Mouse brain imaging using photoacoustic computed tomography. Proc. SPIE 8943, Photons Plus Ultrasound: Imaging and Sensing 2014, 894340. <https://doi.org/10.1117/12.2039669>
- [151.]Zhang P, Li L, Lin L, Hu P, Shi J, He Y, Zhu L, Zhou Y, Wang LV (2018) High-resolution deep functional imaging of the whole mouse brain by photoacoustic computed tomography in vivo. J Biophotonics 11(1). <https://doi.org/10.1002/jbio.201700024>
- [152.]Bell MAL, Ostrowski AK, Kazanides P, Boctor E (2014) Feasibility of transcranial photoacoustic imaging for interventional guidance of endonasal surgeries. Proc. SPIE 8943, Photons Plus Ultrasound: Imaging and Sensing 2014, 894307. <https://doi.org/10.1117/12.2038511>
- [153.]Liu X, Duan Y, Liu B (2021) Nanoparticles as contrast agents for photoacoustic brain imaging. Aggregate 2(1): 4–19. <https://doi.org/10.1002/agt.2.26>
- [154.]Kang J, Zhang HK, Kadam SD, Fedorko J, Valentine H, Malla AP, Yan P, Harraz MM, Kang JU, Rahmim A, Gjedde A, Loew LM, Wong DF, Boctor EM (2019) Transcranial Recording of Electrophysiological Neural Activity in the Rodent Brain in vivo Using Functional Photoacoustic Imaging of Near-Infrared Voltage-Sensitive Dye. Frontiers in Neuroscience 13(579). <https://doi.org/10.3389/fnins.2019.00579>
- [155.]Tang J, Dai X, Jiang H (2016) Wearable scanning photoacoustic brain imaging in behaving rats. J Biophotonics 9(6): 570–575. <https://doi.org/10.1002/jbio.201500311>
- [156.]Tang J, Coleman JE, Dai X, Jiang H (2016) Wearable 3-D Photoacoustic Tomography for Functional Brain Imaging in Behaving Rats. Scientific Reports 6: 25470. <https://doi.org/10.1038/srep25470>
- [157.]Tang J (2016) Photoacoustic Brain Imaging in Behaving Animals. A dissertation presented in partial fulfillment of the requirements for the degree of doctor of philosophy, university of Florida. URL (Last seen in 30th Aug. 2021): <https://ufdc.ufl.edu/UFE0049839/00001>

- [158.] Li L, Zhu L, Ma C, Lin L, Yao J, Wang L, Maslov K, Zhang R, Chen W, Shi J, Wang LV (2017) Single-impulse panoramic photoacoustic computed tomography of small-animal whole-body dynamics at high spatiotemporal resolution. *Nat Biomed Eng* 1: 0071. <https://doi.org/10.1038/s41551-017-0071>
- [159.] Hariri A, Tavakoli E, Adabi S, Gelovani J, Avnani MRN (2017) Functional photoacoustic tomography for neonatal brain imaging: developments and challenges. *Photons Plus Ultrasound: Imaging and Sensing 2017*, Proc. of SPIE Vol. 10064, 100642Z. <https://doi.org/10.1117/12.2254861>
- [160.] Liang B, Liu W, Zhan Q, Li M, Zhuang M, Liu QH, Yao J (2019) Impacts of the murine skull on high-frequency transcranial photoacoustic brain imaging. *J Biophotonics* 12(7): e201800466. <https://doi.org/10.1002/jbio.201800466>
- [161.] Hartman RK, Hallam KA, Donnelly EM, Emelianov SY (2019) Photoacoustic imaging of gold nanorods in the brain delivered via microbubble-assisted focused ultrasound: a tool for in vivo molecular neuroimaging. *Laser Phys Lett* 16(2):025603. <https://doi.org/10.1088/1612-202x/aaf89e>
- [162.] Lv J, Li S, Zhang J, Duan F, Wu Z, Chen R, Chen M, Huang S, Ma H, Nie L (2020) In vivo photoacoustic imaging dynamically monitors the structural and functional changes of ischemic stroke at a very early stage. *Theranostics* 10(2):816-828. <https://doi.org/10.7150/thno.38554>
- [163.] Jolesz FA (2014) Introduction. In: Jolesz F. (eds) *Intraoperative Imaging and Image-Guided Therapy*. Springer, New York, NY. https://doi.org/10.1007/978-1-4614-7657-3_1
- [164.] Han SH (2018) Review of Photoacoustic Imaging for Imaging-Guided Spinal Surgery. *Neurospine* 15(4): 306-322. <https://doi.org/10.14245/ns.1836206.103>
- [165.] Kosik I, Brackstone M, Kornecki A, Chamson-Reig A, Wong P, Araghi MH, Carson JJ (2019) Intraoperative photoacoustic screening of breast cancer: a new perspective on malignancy visualization and surgical guidance. *J of Biomedical Optics* 24(5): 056002. <https://doi.org/10.1117/1.jbo.24.5.056002>
- [166.] Bell M, Boctor E, Kazanzides P (2020) method and system for transcranial photoacoustic imaging for guiding skull base surgeries. US Patent No. 10,531,828 B2. (US010531828B2) Appl. No. 14/611,628.
- [167.] Wiacek A, Bell MAL (1 April 2021) Photoacoustic-guided surgery from head to toe [Invited]. *Biomedical Optics Express* 12(4). <https://doi.org/10.1364/BOE.417984>
- [168.] Haar GT (2016) HIFU Tissue Ablation: Concept and Devices. Ch. 1 in: *Therapeutic Ultrasound*, edited by: Escoffre J-M and Bouakaz A, *Advances in Experimental Medicine and Biology*, Vol. 880, Springer International Publishing Switzerland. https://doi.org/10.1007/978-3-319-22536-4_1
- [169.] Farhanieh O, Sahafi A, Bardhan Roy R, Ergun AS, Bozkurt A (2017) Integrated HIFU Drive System on a Chip for CMUT-Based Catheter Ablation System. *IEEE Transactions on Biomedical Circuits and Systems*. 11(3): 534-546. <https://doi.org/10.1109/TBCAS.2017.2649942>
- [170.] Almekkawy M, Ebbini E (2020) The Optimization of Transcostal Phased Array Refocusing Using the Semidefinite Relaxation Method. *IEEE Transactions on Ultrasonics, Ferroelectrics, and Frequency Control*. 67(2): 318 – 328. <https://doi.org/10.1109/TUFFC.2019.2944434>
- [171.] Funke AR, Aubry J-F, Fink M, Boccara A-C, Bossy E (2009) Photoacoustic guidance of high intensity focused ultrasound with selective optical contrasts and time-reversal. *Applied Physics Letters* 94: 054102. <https://doi.org/10.1063/1.3077018>
- [172.] Cui H, Staley J, Yang X (2010) Integration of photoacoustic imaging and high-intensity focused ultrasound. *J of Biomed Optics* 15(2): 021312. <https://doi.org/10.1117/1.3365948>
- [173.] Sun Y, O'Neill B (2013) Imaging high-intensity focused ultrasound-induced tissue denaturation by multispectral photoacoustic method: an ex vivo study. *Applied Optics* 52(8): 1764-1770. <https://doi.org/10.1364/ao.52.001764>
- [174.] Nguyen VP, Kim J, Ha KL, Oh J, Kang HW (2014) Feasibility study on photoacoustic guidance for high-intensity focused ultrasound-induced hemostasis. *Journal of Biomedical Optics* 19(10): 105010. <https://doi.org/10.1117/1.jbo.19.10.105010>
- [175.] GadAllah MT, Badawy SM (2014) A Wavelet Based Approach for Ultrasound Image Restoration. *IJACSA* 5(7). <https://dx.doi.org/10.14569/IJACSA.2014.050704>
- [176.] Szabo TL (2014) Introduction; Ch.1. and Ultrasound-induced Bioeffects; Ch 15. In: *Diagnostic Ultrasound Imaging: Inside Out*, Second Edition 2014 (by: Szabo TL), Elsevier Inc. <https://doi.org/10.1016/C2011-0-07261-7>
- [177.] Yadollahpour A, Rashidi S (2017) A review of mechanism of actions of ultrasound waves for treatment of soft tissue injuries. *International Journal of Green Pharmacy* 11(1). <http://dx.doi.org/10.22377/ijgp.v11i01.870>
- [178.] Ter Haar GR (2011) Ultrasonic imaging: safety considerations. *Interface Focus* 1(4): 686-697. <https://doi.org/10.1098/rsfs.2011.0029>
- [179.] Ter Haar GR (2010) Ultrasound bioeffects and safety. *Proc Inst Mech Eng H* 224(2): 363-673. <https://doi.org/10.1243/09544119jeim613>
- [180.] Ter Haar GR (2004) Assessment of Possible Hazard in Use; Ch. 14. In: *Physical Principles of Medical Ultrasonics*, 2nd Edition 2004, edited by: Hill CR, Bamber JC and Ter Haar GR, John Wiley & Sons Ltd. <https://doi.org/10.1002/0470093978.ch14>
- [181.] Izadifar Z, Babyn P, Chapman D (2017) Mechanical and Biological Effects of Ultrasound: A Review of Present Knowledge. *Ultrasound Med Biol* 43(6): 1085-1104. <https://doi.org/10.1016/j.ultrasmedbio.2017.01.023>
- [182.] Sliney DH, Trokel SL (1993) Safety Standards and Laser Exposure Limits; Ch. 6. Pp 87-97. In: *Medical Lasers and Their Safe Use*. Springer, New York, NY. https://doi.org/10.1007/978-1-4613-9252-1_6
- [183.] Smalley PJ (2013) Laser safety: regulations, standards, and guidelines for practice. Ch. 24. Pp. 725-759. In: *Lasers for medical applications - Diagnostics, therapy and surgery*. Edited by Jelínková H. Woodhead Pub. Ltd. <https://doi.org/10.1533/9780857097545.4.725>
- [184.] Kim J, Choi W, Park E-Y, Kang Y, Lee KJ, Kim HH, Kim WJ, Kim C (Dec. 2019) Real-time Photoacoustic Thermometry Combined with Clinical Ultrasound Imaging and High Intensity Focused Ultrasound. *IEEE TBME* 66(12): 3330 - 3338. <https://doi.org/10.1109/TBME.2019.2904087>
- [185.] Joa J, Tianb C, Xuc G, Sarazind J, Schiopud E, Gandikotac G, Wang X (2018) Photoacoustic tomography for human musculoskeletal imaging and inflammatory arthritis detection. *Photoacoustics* 12. <https://doi.org/10.1016/j.pacs.2018.07.004>
- [186.] Yagi T (2018) Photoacoustic Imaging: Opens a Door to the Future. *ImPACT*. URL (Last seen in Aug. 30th, 2021): https://www.jst.go.jp/impact/hp_yagi/progress/booklet_e.pdf
- [187.] Lengenfelder B, Mehari F, Hohmann M, Heinlein M, Chelales E, Waldner MJ, Klämpfl F, Zalevsky Z, Schmidt M (2019) Remote photoacoustic sensing using speckle-analysis. *Scientific Reports* 9: 1057. <https://doi.org/10.1038/s41598-018-38446-x>
- [188.] Meng L, Deschaume O, Larbanoix L, Fron E, Bartic C, Laurent S, Van der Auweraer M, Glorieux C (2019) Photoacoustic temperature imaging based on multi-wavelength excitation. *Photoacoustics* 13: 33-45. <https://doi.org/10.1016/j.pacs.2018.11.004>
- [189.] Martinho Costa M, Shah A, Rivens I, Box C, O'Shea T, Papaevangelou E, Bamber J, Ter Haar G (2019) Quantitative photoacoustic imaging study of tumours in vivo: Baseline variations in quantitative measurements. *Photoacoustics* 13:53-65. <https://doi.org/10.1016/j.pacs.2018.12.002>

Arabic Title:

التصوير الصوتي الضوئي في الطب – مراجعة

Arabic Abstract:

بدأت هذه الورقة البحثية الخاصة بالتصوير الصوتي الضوئي (PAI) في الطب بمقدمة للتصوير الصوتي الضوئي والتقنيات الصوتية الضوئية الشهيرة بما في ذلك التصوير المقطعي الصوتي الضوئي (PAT)، والتصوير المقطعي الصوتي متعدد الأطياف (MSOT)، والفحص المجهرية الصوتي الضوئي (PAM)، والتنظير النقطي الصوتي الضوئي (RSOM)، وتصوير المرونة الصوتي الضوئي (PAE). تم أيضاً عرض مراجعة متواضعة حول الموجات فوق الصوتية بالليزر بدون تلامس (LUS)، والتي تتمتع بميزة جودة الصورة المستقلة عن المشغل، كما يتم عرض مراجعة موجزة لمعظم التطبيقات الطبية للتصوير الصوتي الضوئي بما في ذلك فحص السرطان (للثدي والغدة الدرقية والمبيض والبروستاتا والرئة والجلد)، وقياسات أكسجة الأنسجة، وتصوير الدماغ، والجراحة الموجهة بالتصوير (IGS)، وتوجيه الموجات فوق الصوتية المركزة (HIFU). بعد ذلك تم تقديم بعض اعتبارات السلامة المتعلقة باستخدام الموجات فوق الصوتية الطبية والليزر. وفي الختام، من المتوقع المزيد من التطوير العلمي والسريبي في مجال PAI، ومن المتوقع أيضاً أن تخدم زيادة الأجهزة المعتمدة التي تستخدم تقنيات PAI في التطبيقات الطبية قطاعات واسعة من الطب، سواء كانت تشخيصية أو علاجية.

AUTHORS' BIOGRAPHIES



Mohammed Tarek GadAllah is now an Assistant Researcher with Computers and Systems Department, Electronics Research Institute (ERI), Egypt. He joined ERI in July 19th, 2016. Mohammed was born in Menoufia, Egypt, in Dec. 29, 1986. He was awarded the Degree of Bachelor of Electronic Engineering in July 29th, 2008 from Industrial Electronics and Control Engineering Department, Faculty of Electronic Engineering, Menoufia University, Egypt. He was awarded the Degree of Master in Electronic Engineering in Feb. 23th, 2015 from Control Systems and Measurements Engineering Department, Faculty of Electronic Engineering, Menoufia University, Egypt. Mohammed has more than one achievement in designing and fabricating electronic circuits. He is now a post-graduate – Ph.D. student with Industrial Electronics and Control Engineering Department, Faculty of Electronic Engineering, Menoufia University, Egypt. His previous and current research interests include: Ultrasound Imaging, Photoacoustic Imaging, Digital Image Processing, Medical Imaging, Electronic Circuits, Biomedical Engineering, and Electronics Engineering. His Web of Science **Researcher-ID** is: [N-7825-2013](https://publons.com/a/2579422) (<https://publons.com/a/2579422>). His **ORCID** is: <https://orcid.org/0000-0002-9353-3986>.
E-mails: mohammed.tag.1986@eri.sci.eg; mohammed.tag.1986@gmail.com.



Abd El-Naser Abd El-Gawad Mohamed is now a Professor Emeritus with Electronics and Electrical Communications Engineering Department, Faculty of Electronic Engineering, Menoufia University, Egypt. He awarded his Ph.D. in 1994 from Menoufia University. His previous and current research interests are in the area of optical communications (Optical Sources, Detectors, Optical amplifiers, Optical cables, Optical networks, Optical computers, Optical measurements, Optical connectors, Different propagation phenomena in different optical channels, ... etc.), and the area of digital communication systems.
E-mail: abd_elnaser6@yahoo.com.



Alaa Abd El-Fattah Hefnawy is a Professor at the Electronics Research Institute, Cairo, Egypt. He joined the Electronics Research Institute in 1993, and he headed the Computer & Systems Dept. for four years (2013-2017). His department has five main research groups; the digital signal processing group, the biometrics group, the high-performance processing group, the artificial intelligent group, and the computer network group. Professor Hefnawy

supervised all the research and academic activities of his 77 Faculties, Phd, and MSc students in his Dept. including the currently running research projects. His fields of interest are digital communications, digital signal processing, biometrics, image/speech coding, image indexing and retrieval, pattern recognition and machine vision. Prof. Hefnawy received his B. Sc., M. Sc., and Ph. D. in Electronics and Electrical Communications from Faculty of Engineering, Cairo University in 1992, 1995 and 2000 respectively. He was a visiting professor at UBC, Canada in 2015, at Kobe Univ., Japan, twice in 2007 & 2014, and a visiting fellow at Brno Univ. of Technology, Czech, in 2012, and at the Univ. of Texas at Austin (USA), in 2011. Prof. Hefnawy has joined the Ministry of communications and Information Technology of Egypt in 2005 till 2007, as IT Project Manager. He participated also as an Outreach and Implementation Consultant, under the United Nation Development Program (UNDP). He has many publications in his scientific fields, supervised many master and Ph. D. thesis, and attended more than 16 international conferences around all over the world. Prof. Hefnawy has a wide teaching experience for more than 24 years. He has been teaching and enhancing courses in Electrical Communications Engineering and some other conducted and developed custom short courses, for both undergraduate and postgraduate students. He was teaching in many places; Cairo University, Misr University for Science & Technology, October 6 University, American University in Cairo, and Eltaief University & ArabEast College for postgraduate (KSA).

E-mails: alaa@eri.sci.eg; alaahouse@yahoo.com.



Hassan EL-Banna Zidan is a researcher in the Electronics Research Institute (ERI), Cairo, Egypt, since 2015. He got his Ph.D. from the Norwegian university of science and technology (NTNU), Trondheim, Norway 2014 and his master's degree from the Arab Academy of science technology and maritime transport (AASTMT), Cairo, Egypt 2007. His research interests include acoustics, audio, speech and image signal processing. His **ORCID** is: <https://orcid.org/0000-0002-5529-9519>.
E-mails: hbanna@eri.sci.eg; hbanna@gmail.com.



Ghada Mohammed El-Banby received the M.Sc. and Ph.D. degrees in Automatic Control Engineering from Menoufia University, Egypt in 2006, and 2012, respectively. Currently she is working as Associative Professor at the Department of Industrial Electronics and Control Engineering, Faculty of Electronic Engineering, Menoufia University. Her current research interests include computer vision, data fusion, image processing, signal processing, medical imaging, modeling, and control. Her **ORCID** is: <https://orcid.org/0000-0002-7789-9195>.
E-mail: ghadaelbanby75@gmail.com.



Samir Mohammed Badawy; Professor Emeritus, Industrial Electronics, and Control Engineering Department, Faculty of Electronic Engineering, Menoufia University, Egypt. Dr. Badawy received his Ph.D. degree from the Institute of cancer research, Royal Marsden Hospital, London University, UK. He received his Master's Degree from Helwan University,

Egypt. He was awarded the Degree of Bachelor of Engineering from Industrial Electronics Department, Faculty of Engineering, Menoufia University, Egypt. His previous and current research interests include Biomedical Physics, Biomedical Electronics, BCI, EYE Computer and system interface (ECI), Medical Image Processing, Enhancement and Analysis, Ultrasound Tissue Characterization and Reconstruction, and Biological Magnetic Effects on Living Cells.

Ex: Ajman University of science and technology advisory board member, dean of faculty of engineering, head, and establisher of the biomedical engineering department, head of the conferences and seminars group.

E-mails: drsamirb@gmail.com; Samir.badawy@el-eng.menofia.edu.